

KM9106

Operators Manual


CONTENTS

	Page No:
1. ANALYSER LAYOUT AND FEATURES	1
1.1 Handset features	1
1.2 Analyser features.....	2
1.3 Standard Probe Configuration.....	3
1.4 Analyser connections	4
2. SAFETY WARNING	5
3. FIRST TIME USE	5
4. NORMAL START UP SEQUENCE.....	6
4.1 Every Time you use the Analyser	6
4.2 Automatic Calibration.....	6
4.3 Main Display Parameters	8
4.3.1 Page Mode.....	8
4.3.2 Line Scroll Mode	9
4.4 Sampling the Flue Gas	10
4.5 Taking a Pressure Reading.....	11
4.6 Regular Checks During Sampling.....	11
4.7 Normal Shutdown Sequence	12
4.8 Electromagnetic Compatibility	12
4.9 HC104 Module.....	12
5. USING THE KEYPAD.....	13
5.1 Basic Operation.....	13
5.2 Quick Key Operations.....	13
5.3 Display Hold	14
5.4 Display Backlight and Contrast	15
5.5 Pump	15
6. USER SELECTABLE SETTINGS.....	16
6.1 Time and Date	17
6.2 Changing a Fuel	18
6.3 Gross or Nett Efficiency.....	20
6.4 Scale Options	21
6.5 Inlet Temperatures	26
6.6 Oxygen Calibration	27
6.7 Toxic sensor Zero.....	27
6.8 CO Alarm.....	29


7. PRINTING INFORMATION	30
7.1 Changing Printout Parameters	31
7.2 User Defined Printouts	33
7.2.1 Standard Printout	34
7.2.2 Master List of Printed Parameters	35
8. QUINTOX LOGGING AND PC DOWNLOAD	36
8.1 Overview	36
8.1.1 Description	36
8.1.2 Switching the Logger on	36
8.1.3 Logging Data	37
8.2 Batteries	37
8.3 Logger Control	38
8.4 Downloading Information	40
8.4.1 Setting Up your PC	41
8.4.2 Capturing Data from Quintox	42
8.4.3 Downloading Logged Data	42
9. CONTINUOUS MONITORING	43
10. MAIN PURGE	44
11. MAINTENANCE	47
11.1 Emptying and Cleaning the In-line Water Trap	47
11.2 Changing the Particle Filter	47
11.3 Charging the Battery	48
11.4 Changing the Paper Roll	48
11.5 Changing the Printer Ribbon	49
12. PROBLEM SOLVING	50
13. ANNUAL RE-CALIBRATION	51
14. HOW TO GET EXPERT HELP	52
15. PRODUCT SPECIFICATION	53
APPENDICES:	56
A. MAIN DISPLAY PARAMETERS	56
B. NO _x CALCULATIONS	60
C. COMBUSTION EFFICIENCY CALCULATION	63
D. CALCULATION OF FUEL DATA	65
E. ELECTROMAGNETIC CAPATIBILITY STATEMENT	66

1. ANALYSER LAYOUT AND FEATURES

1.1 Handset Features

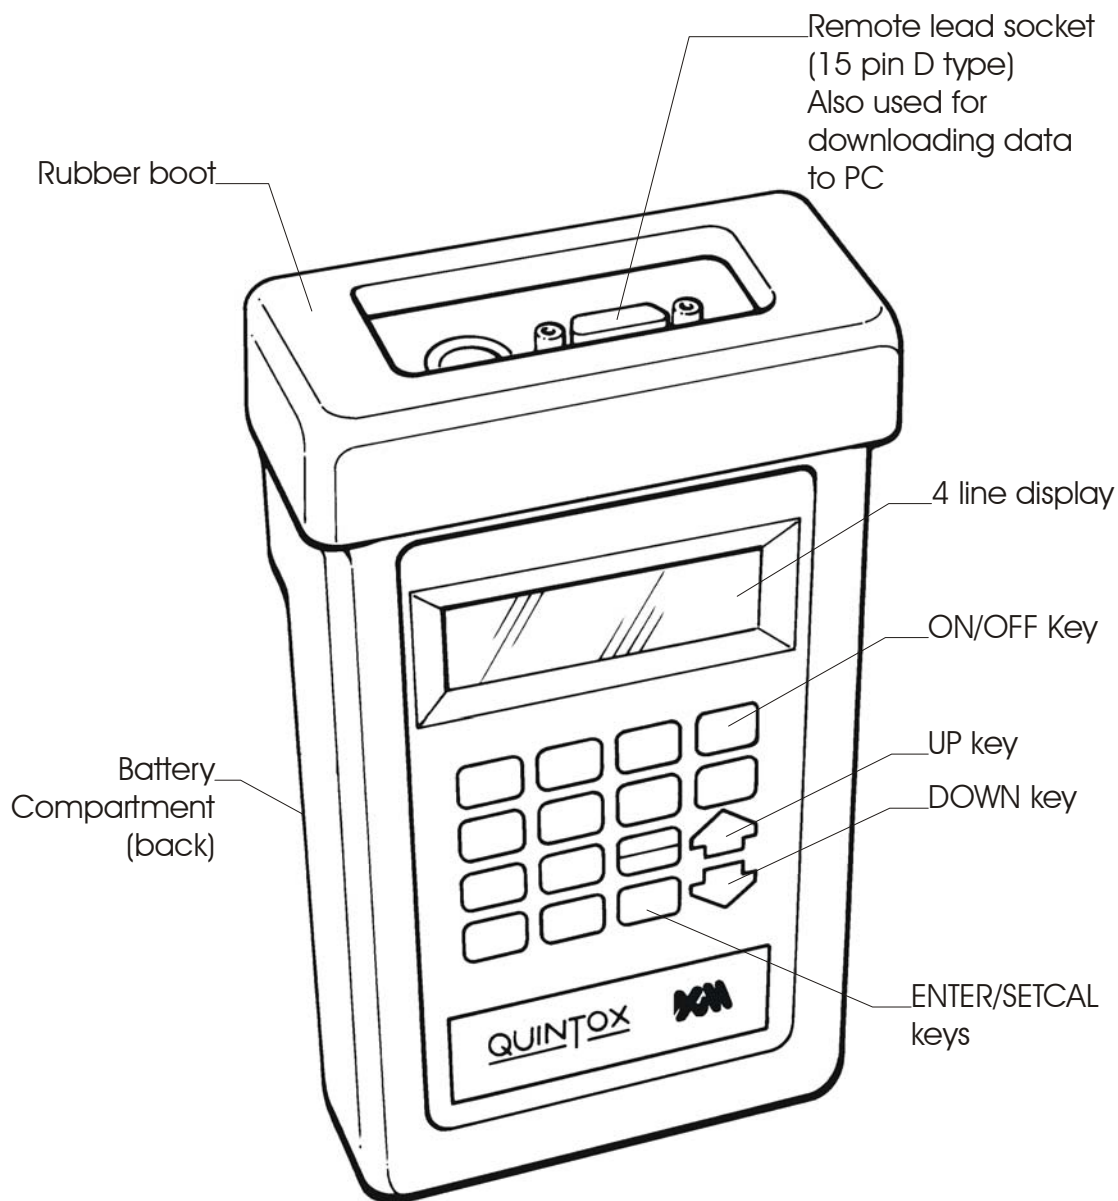

Commonly used keys



ON/OFF



UP

Pages up through screens
Scrolls up through options, ie Fuel



ENTER & SET/CAL


Accepts parameters
Enters values




DOWN

Pages down through screens
Scrolls down through options


1.2 Analyser Layout

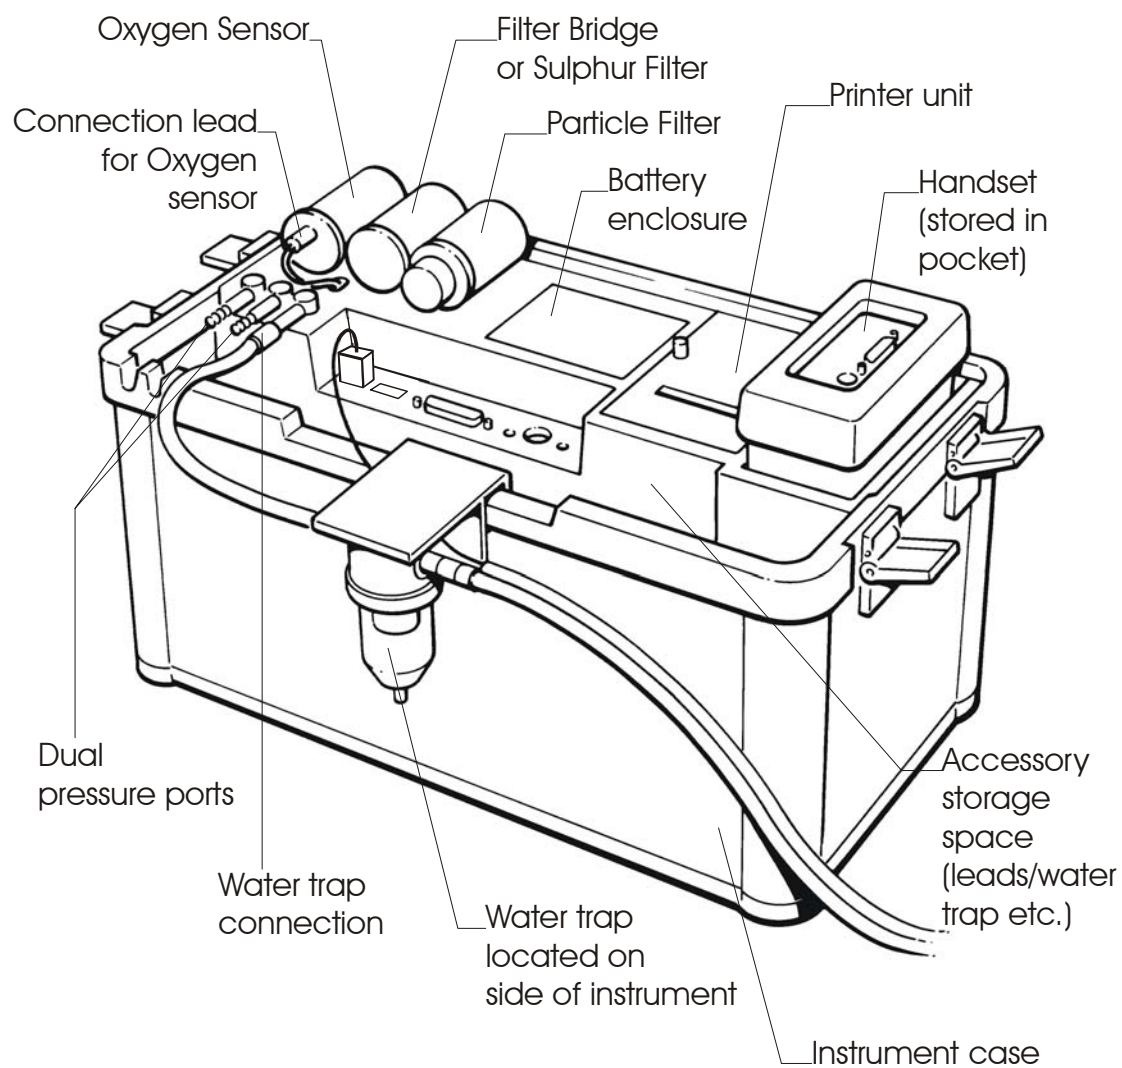

1.3 Standard Probe Configuration

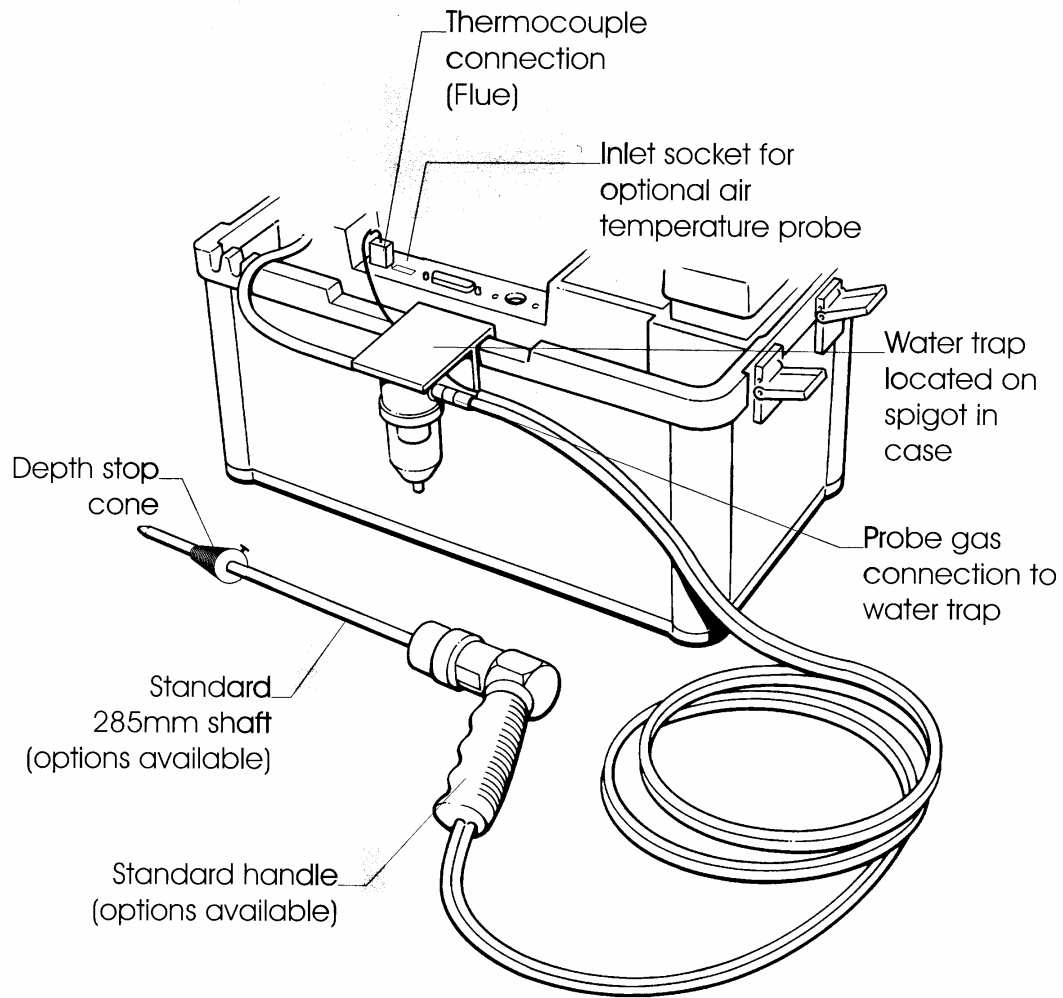

1.4 Analyser Connections

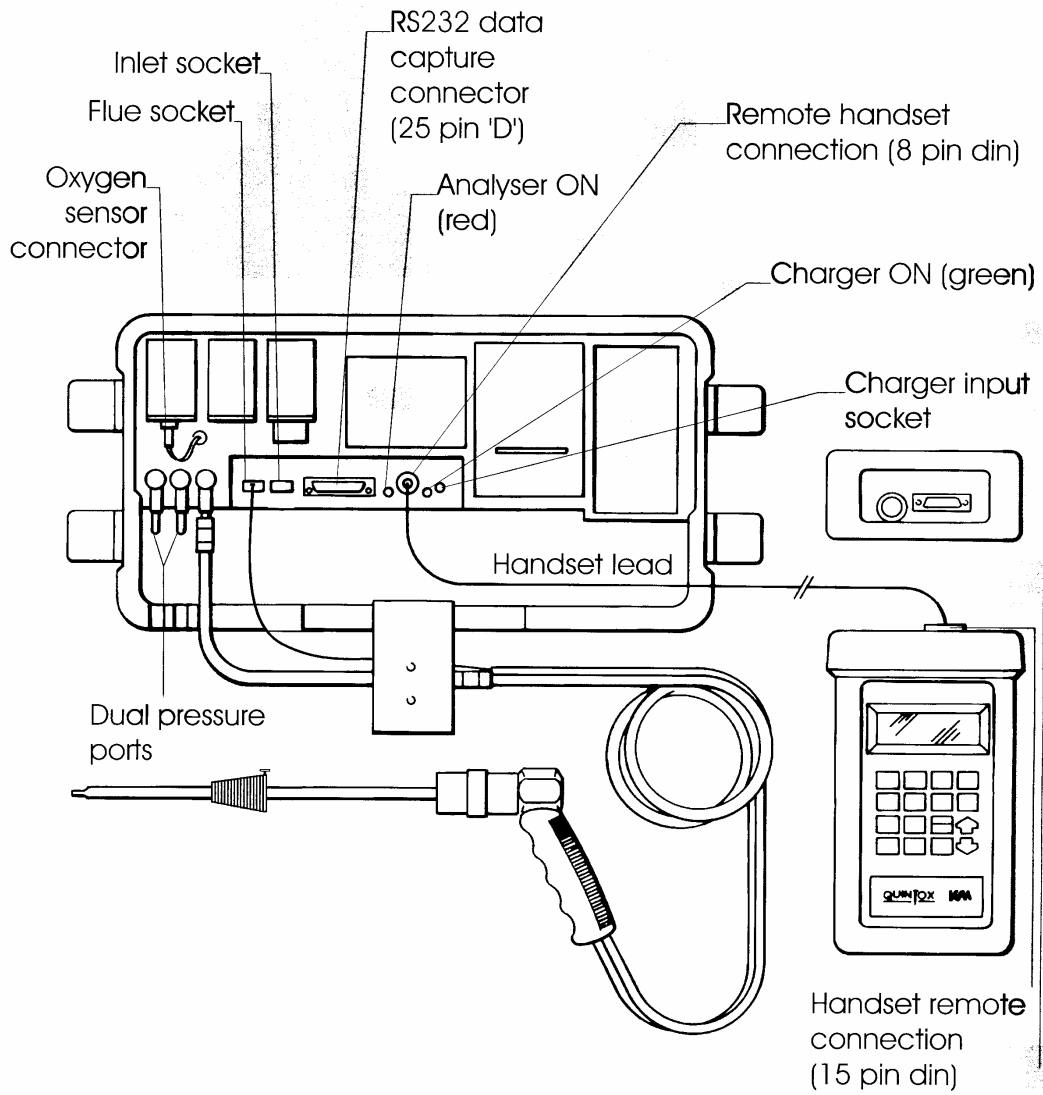



2. SAFETY WARNING

This analyser extracts combustion gases that may be toxic in relatively low concentrations. These gases are exhausted from the bottom of the instrument. This instrument must only be used in well ventilated locations. It must only be used by trained and competent persons after due consideration of all the potential hazards.

3. FIRST TIME USE

Charge the battery for 12 hours, following this an overnight charge should be sufficient for an average 8 hour day.

Whilst charging the green LED will be illuminated, the LED will flash when the battery is fully charged.

Check that you have all the items you have ordered.

We offer a wide choice of probes which are not supplied as standard and must be ordered as a separate item.

Take time to read this manual fully.

TIP: Take a look at the Spare Parts list and order some replacement filters and paper rolls now.

When using the analyser for the first time you have the following under your control

PARAMETER	SECTION
Display Contrast	5.4
Backlight	5.4
Language	6.4
Line Rejection for mains frequency	6.4
Gas Measurement Scale	6.4
Temperature scale	6.4
Pressure scale	6.4
Reference oxygen	6.4
Time and date	6.1
Printed header name and telephone number	7.1

4. NORMAL START UP SEQUENCE

4.1 Every Time You Use The Analyser

BEFORE SWITCH-ON CHECK THAT:

- the Oxygen sensor is connected
- the particle filter is not dirty
- the sulphur filter is fitted for heavy oil or coal
- the water trap and probe line are empty of water
- all hose connections, etc, are properly made
- the paper roll is fitted
- the probe is sampling ambient FRESH air
- the water trap is vertical
- the flue temperature is connected
- the instrument is placed on a clean, flat, level surface

Switch ON the instrument by pressing



4.2 Automatic Calibration



During this sequence the analyser pumps fresh air into the sensors to allow toxic sensors to be set to zero and the Oxygen sensor to be set to 20.9 %.

After switch-on the analyser will briefly display the Kane logo and telephone numbers:-

*** KANE-MAY ***
TEL +44 (0) 1707 375550
FAX +44 (0) 1707 393277

Followed by the logger menu screen :-

* * SELECT FUNCTION * *
1 . . LOGGER CONTROL
2 . . QUINTOX CONTROL

Use the  and  keys to position the cursor over 2 . . Quintox Control.

Press  to access Quintox Control

* * SELECT FUNCTION * *
1 . . LOGGER CONTROL
2 . . QUINTOX CONTROL

And show the countdown screen :-




The display will countdown from 300 to zero in one second steps. If the analyser has been used recently it may complete automatic calibration in less than 300 seconds otherwise it will count to zero.

Once the calibration sequence is complete an audible beep will be heard and will show the selected fuel on the following display:-



Press 


This zeros the toxic sensor and sets Oxygen to 20.9%. The next screen is the **MAIN DISPLAY** of the analyser:-

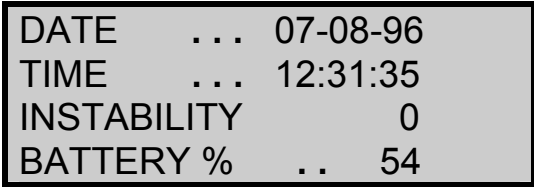

MAIN DISPLAY

NOTE : It is advisable to repeat Oxygen Calibration every 2 hours for maximum accuracy.

Use  and  to change the display.

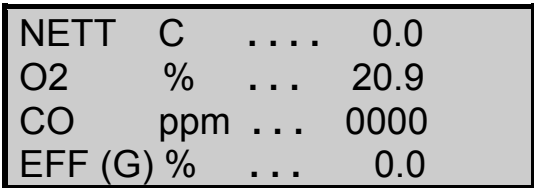


All parameters are detailed in Appendix A - MAIN DISPLAY PARAMETERS.

4.3 Main Displays



The main display can be changed to show the following :-

- **Page Mode** displays 4 lines of data in set format, each page is predefined.
- **Line scroll mode** allows you to customise the display with the data you require.

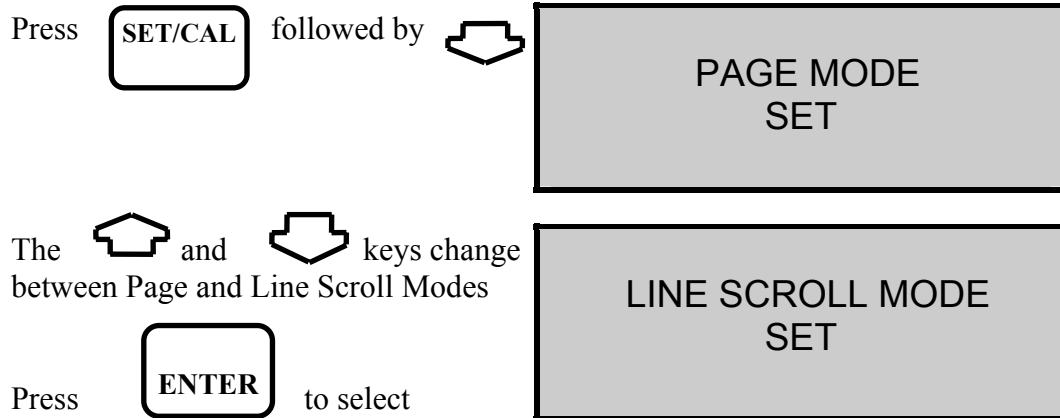To change between the different modes :-



4.3.1 Page Mode

Use the  and  keys to change the information displayed on the screen. The following are a number of the pages available. Other parameters on other screens are detailed in Appendix A.

NETT	C	...	0.0
O2	%	...	20.9
CO	ppm	..	0000
EFF (G)	%	...	0.0

CO2	%	...	0.0
FLUE	C	...	0.0
INLT			NOT FITTED
AMBIENT	C	...	21



CO/CO2	R	..	0.0001
P INDEX	%	...	0.01
XAIR	%	...	0.0
Prs	mbar		0.00


This screen only shows readings if optional sensors are fitted. In this instance the SO2 sensor is NOT FITTED.

NO	ppm	..	0000
NO2	ppm	..	0000
NOx	ppm	..	0000
SO2			NOT FITTED


4.3.2 Line Scroll Mode

Line scroll mode allows you to customise the display.

Use the  key to change the bottom line of the display. Once the correct line is displayed press  to confirm and move the line up. Select the next parameter and repeat until all lines display the desired parameters.

Change bottom line using 

NETT	C	...	0.0
O2	%	...	20.9
CO	ppm	..	0000
CO2	%	...	0.0

to select and move parameter up 

O2	%	...	20.9
CO	ppm	..	0000
CO2	%	...	0.0
CO2	%	...	0.0


Select next parameter.
Repeat above until
display reads desired data

O2	%	...	20.9
CO	ppm	..	0000
CO2	%	...	0.0
CO/CO2 R	..		0.0001

4.4 Sampling the Flue Gas

Once the automatic calibration procedure has been completed and the specific fuel has been selected the probe can be inserted into the desired sampling point.

It is recommended that the sampling point be located at least two flue diameters downstream of any bend and that the probe tip is in the centre of the flue (this is normally the point of the hottest temperature). With balanced flues and other domestic units the probe should be positioned far enough into the flue so that no air can 'back flush' into the probe.

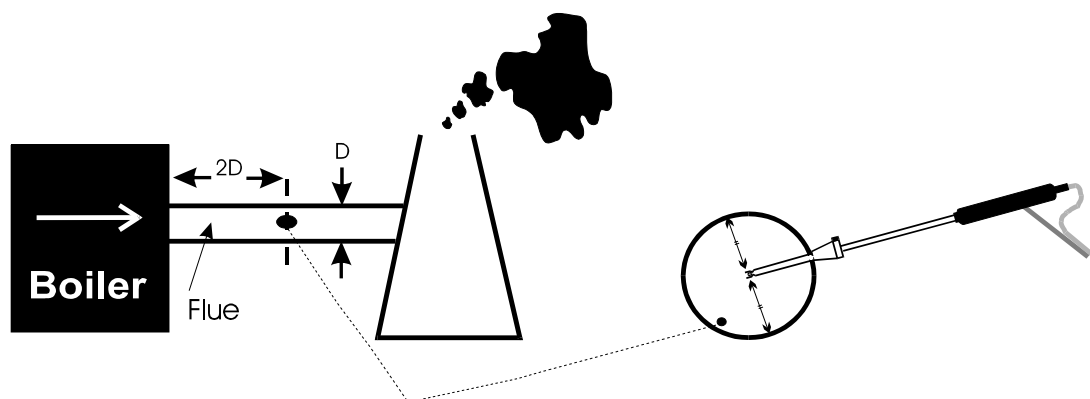

The probe depth stop cone provided with the instrument allows the probe to be used in holes whose diameters range from 8 mm to 21 mm ($\frac{5}{16}$ to $\frac{4}{5}$ inch).

The standard probe is rated at 650°C/1202°F. Temperatures of up to 1100°C/2012°F can be accommodated using an optional high temperature probe.

TIP: To conserve battery power, switch off the pump when you are not taking a measurement. Use the


PUMP

4.5 Taking a Pressure Reading

With the optional pressure module fitted a flue draught measurement can be made at any time.

Connect the standard probe to the appropriate pressure sensor inlet and place the probe in the flue.

The pressure reading will be displayed :-

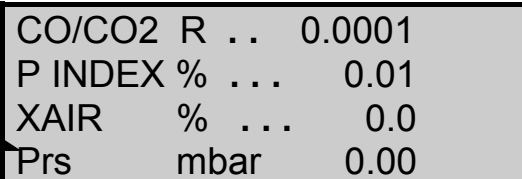

CO/CO2 R ..	0.0001
P INDEX % ...	0.01
XAIR % ...	0.0
Prs mbar	0.00

NOTE: Care must be taken to connect the probe to the correct port as the pressure will be displayed in reverse i.e. a positive pressure rather than negative draught.

To perform a combustion test and display draught pressure at the same time a special probe is required. Contact Kane International or Authorised Distributor for details.

Two pressure ports are provided on the instrument for use with a Pitot tube. Contact Kane International Ltd. for details of this probe and its availability.

4.6 Regular Checks During Sampling

Care must be taken at all times not to exceed the analyser's operating specification. In particular ensure the following :-

- Do not exceed the maximum temperature of the flue probe.
- The analyser's internal temperature does not exceed normal operating range, typically 0-40°C.
- DO NOT PLACE THE ANALYSER ON A HOT SURFACE.
- The water trap is vertical at all times. Water condenses in the probe line and can quickly fill the water trap when the probe is moved. Take care and watch the water trap closely.
- The in-line particle filter is clean and does not become blocked.

4.7 Normal Shutdown Sequence

DO THIS EVERY TIME YOU USE THE ANALYSER.

Remove the probe from the flue - **TAKE CARE ! THE PROBE WILL BE HOT** - and allow it to cool naturally. Do not immerse the probe in water as this will be drawn into the analyser and damage the pump and sensors.

Once the probe is removed from the flue, the oxygen reading 20.9% and the CO reading is zero press



and the analyser will switch off.

Check the water trap and probe tubes for water before packing away.

4.8 Electromagnetic Compatibility

The European Council Directive 89/336/EEC requires that electronic equipment does not generate electromagnetic disturbances that exceed defined levels and has an adequate level of immunity to enable it to be operated as intended. The specific standards applicable to this product are detailed in the appendices.

Since there are many electrical products in use that pre-date this Directive and may emit electromagnetic radiation in excess of the standards defined in the Directive there may be occasions where it would be appropriate to check the analyser prior to use. The following procedure should be adopted:

Go through the normal start up sequence in the location where the equipment is to be used.

Switch on all localised electrical equipment that might be capable of causing interference.

Check that all readings are as expected. (A level of disturbance in the readings is acceptable). If not adjust the position of the instrument to minimise interference or switch off, if possible, the offending equipment for the duration of the test.

N.B. Maximum cable lengths must be less than 3 metres.

At the time of writing this manual (January 1997) Kane International Ltd is not aware of any field based situation where such interference has ever occurred and this advice is only given to satisfy the requirements of the Directive.

4.9 HC104 Module

With this module fitted and working the CO₂ value is always the measured value not the calculated value. The handset display and print out indicate that the CO₂ value is a measured value by showing CO₂m. If the module is not fitted, the KM9106 automatically defaults to calculated CO₂. If during start up calibration a fault is detected in the CO₂ module, the instrument will default to calculated. If the instrument displays CO₂m FAULT during operation, by switching OFF and then ON, the instrument will default to calculated CO₂.

5. USING THE KEYPAD

5.1 Basic Operation


Basic operation of the keypad to change the display in PAGE and LINE SCROLL mode is detailed section 4.3. These modes give you the facility to perform the following :-

- **Page Mode** displays 4 lines of data in set format, each page is predefined.
- **Line scroll mode** allows you to customise the display with the data you require.

5.2 QUICK key operation

To allow parameters to be viewed quickly Quintox has a number of QUICK keys. Many of these keys have two functions.

To select an **LOWER PARAMETER** parameter simply press the key i.e.



to display CO₂ and three other


CO2	%	...	20.9
CO	ppm	...	0000
NETT	C	0.0
XAIR		O2 >	20%

To select a **UPPER PARAMETER** parameter press the **UPPER FUNCTION** key



UPPER FUNCTION			

Followed by the **UPPER PARAMETER** you require parameter key i.e. to display NO₂ and three other values



NO2	ppm	0
NO	ppm	0
NETT	C	0.0
CO	ppm	0

Other QUICK keys are detailed below :-

LOWER PARAMETER KEYS

NETT	to display Nett temperature plus O ₂ , CO and Eff.
FLUE	to display Flue temperature plus Ambient, O ₂ and Prs.
INLET	to display Inlet temperature plus Ambient, O ₂ and Flue
O₂	to display Oxygen reading plus CO, CO ₂ and Nett
CO₂	to display Carbon Dioxide calculation or reading CO, Nett and XAIR
CO	to display Carbon Monoxide plus Nett, O ₂ and CO ₂
AUX	to display AUX1 and CxHy readings plus Nett and CO
FUEL	to display chosen fuel and its parameters
EFF	to display Gross efficiency plus O ₂ and CO

UPPER PARAMETER KEYS

ALWAYS Press **UPPER FUNCTION**  first then

SCALE	to display Scaling setup parameters
AMBIENT	to display ambient temperature plus sensor, Flue and Inlet
SO₂	to display Sulphur Dioxide reading plus Nett, O ₂ and CO
NO₂	to display Nitrogen Dioxide reading plus NO, Nett and CO
NO	to display Nitric Oxide reading plus NO _x , Nett and CO
NO_x	to display the Oxides of Nitrogen reading plus NO, CO and Nett
PRESSURE	to display the pressure reading plus Flue, Nett and O ₂
LOSSES	to display all four losses
λ	to display Excess Air plus CO, Eff and CO ₂ .

All measured and calculated values are detailed in Appendix A - Main Display Parameters.

5.3 DISPLAY HOLD

The display hold function allows you to freeze values on the instrument allowing them to be viewed or printed. No measurements are taken once this function has been activated. This feature gives the following benefits :-

- Data can be viewed at a particular point in the boiler tuning process.
- Multiple printouts may be obtained of the same data.
- Scales can be changed between printouts giving different units. i.e. ppm and mg/m³

TO TOGGLE DISPLAY HOLD

Press **UPPER FUNCTION**  followed by 

Indicates the display is held.

#	NETT	C	...	0.0	#
#	O2	%	...	20.9	#
#	CO	ppm	..	0000	#
#	EFF (G)	%	...	0.0	#

In this function only the battery level will be updated and all other parameters are frozen. This does not apply when AUTOPRINT is ON, the time and date are also updated in this mode.

5.4 DISPLAY BACKLIGHT AND CONTRAST


The **display contrast** can be adjusted to suit different lighting conditions and the **backlight** can be switched on or off.

TO TOGGLE THE BACKLIGHT ON /OFF

Press UPPER FUNCTION  followed by 

TO SET THE CONTRAST

Press the  followed by
UPPER FUNCTION key

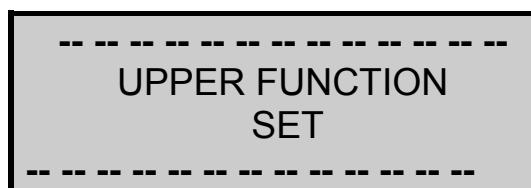

Pressing the  key displays



Hold down either the  or  key and release once the desired level is set.

Press  to confirm setting.

NOTE: The screen may flip from all dark to blank very quickly. Do not panic this is normal - keep pressing the same key until the desired level is displayed.

TIP: **If for any reason the display is not visible at switch on, simply disconnect the handset for a few seconds and re-connect. Then reset the display contrast as detailed above.**

5.5 PUMP

The **Pump** can be toggled on or off from the handset.

TO TOGGLE THE PUMP ON /OFF

Press 

TIP: **When the pump is switched off the O₂ reading will go down as the oxygen sensor consumes the oxygen in its housing!**

6. USER SELECTABLE SETTING

The following features are under your control at any time and can be changed as detailed later in this section.

Time and date	Day/ Month order is selectable and the real time clock and calendar are fully adjustable.
Fuel type	Standard pre-programmed fuels can be selected or users can define their own fuel characteristics.
Efficiency	Efficiency readings can be selected to be based on Gross or Nett values.
Language	The analyser is programmed with ten languages.
Line Rejection	For optimum mains electricity noise rejection a software filter set for either 50 Hz or 60 Hz. Select 50 Hz in Europe and 60 Hz in the USA. Check your country's power frequency.
Gas Scale ppm(n) or mg/m ³ (n)	Normalised or un-normalised ppm or mg/m ³ scalings can be selected. Normalised is also known as referenced readings to Oxygen. See Reference Oxygen below.
Compensation	Some sensors are cross sensitive to other gases. Where appropriate sensors are fitted so this cross sensitivity can be compensated for, improving accuracy. During re-calibration this compensation must be disabled.
Temperature scale	The analyser is programmed for both Celsius and Fahrenheit
Pressure scale	The analyser is programmed for inWG, mBar, cmWG and kPa.
Reference oxygen	Toxic gas measurements can be referenced to defined oxygen levels.
NOx Calculation	Determines the level for calculating NOx. Depends on the sensors fitted and local authority preferences.
Inlet temperature	The flue temperature probe can be used to measure and programme the air inlet temperature to the boiler
Oxygen calibration	If the analyser is being used for multiple checks over the working day it is advisable to re-set the oxygen sensor at regular intervals. This function allows re-set without the need to repeat the start-up routine
Toxic sensor zero	The CO and other optional toxic sensors can be reset to zero if

they drift. This may happen if the sensor is taken to very high concentrations for long periods of time or over-ranged.

6.1 Time and Date (Setting numbers)

This section gives details on setting the time and date and also the general principle of setting a number from 0-9 used in other functions.




TO SET THE TIME AND DATE

Press the  followed by  UPPER FUNCTION key

UPPER FUNCTION
SET

Pressing the  key displays




DAY - MONTH - YEAR
SELECT ORDER

Parameter	Controls	Options
DATE FORMAT:	Select using  or  key and 	DAY-MONTH-YEAR MONTH-DAY-YEAR

To Set The Date:

DATE 26-01-97
SET


Each number in the date is to be set. The cursor under the two in the DAY above indicates this number can be changed. Set each number in the date until correct using the method below, this is also the method for **SETTING NUMBERS**.

Parameter	Controls	Options
DATE:	Select each number using  or  key and 	0 - 9




The cursor moves to each number in turn until the last number is set.

DATE 26-01-97
SET

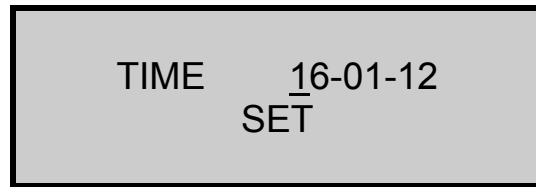To Set The Time:



As with the date each number in the time is to be set.


Parameter	Controls	Options
TIME:	Select each number using  or  key and 	0 - 9

Once the last number has been set the screen will show the main display last shown before entering the set time routine.


6.2 Changing a fuel


This section gives details on changing a standard fuel and entering a user fuel.




TO SET THE FUEL

Press the 



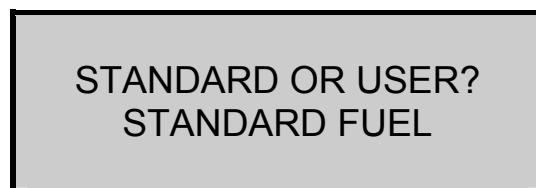Pressing the  key displays






Parameter	Controls	Options
FUEL STANDARD	Select using  or  key and 	STANDARD FUEL USER FUEL




To Set A Standard Fuel:

There are over 70 standard fuels programmed into Quintox. The fuels are arranged into tables for each country and the table should be selected for the origin of the fuel used in your boiler. Each table contains different fuel types, choose the fuel that is closest to the fuel used in your boiler.

SELECT FUEL TABLE
ENGLISH

Parameter	Controls	Options
FUEL TABLE:	Select table for your country using  or  key and 	ENGLISH FRANCAIS DEUTSCH NEDERLANDS ITALIANO CASTELLANO SVENSKA SUOMI OESTERREICH NEW ZEALAND

SELECT FUEL TYPE
NATURAL GAS




Parameter	Controls	Options for English Fuel Table
FUEL TYPE:	Select fuel type using  or  key and 	NATURAL GAS NATURAL GAS 2 TOWN GAS LIGHT OIL HEAVY OIL COAL ANTHRACITE COKE PROPANE BUTANE GASCOR LPG

The table shown above is for the UK. Fuel lists vary depending on the country.

To Set A User Fuel:


If one of the standard fuels does not approximate to the one you are using in your boiler then it is possible to set the Quintox up for a USER FUEL. The information required to be able to set this are the Chemical Breakdown of the fuel and the Gross and Nett calorific value. Details of the calculation are shown in the Appendix.

SET			
K1g	0.350	K1n	0.393
K2	11.89	K3	9.83
K4	32	O2r	3.0

Parameter	Controls	Options
USER FUEL:	Set each number as date using  or  key and 	0 - 9

TIP: If you enter this routine in error, ENTER past all of the numbers to exit.

Check fuel set by pressing



NATURAL GAS			
K1g	0.350	K1n	0.393
K2	11.89	K3	9.83
K4	32	O2r	3.0

6.3 Gross or Net Efficiency


The Quintox can calculate efficiency in of one of two ways.


Efficiency = 100% - Losses. See the Appendix for the Efficiency calculation.

- Gross efficiency uses the gross calorific value of the fuel and deems that the latent heat of vapourisation is lost up the flue of the boiler and is taken as a loss. Gross is used in the UK and USA.
- Net Efficiency uses the net calorific value and assumes the latent heat is not lost up the flue. For Natural gas this efficiency can be 11% higher than the Gross figure. Net is used in France and Germany.

NOTE: Latent heat is the heat required to turn water at 100°C into steam at 100°C, i.e. a change of state from liquid to vapour without rise in temperature has taken place.




TO SET GROSS OR NETT EFFICIENCY

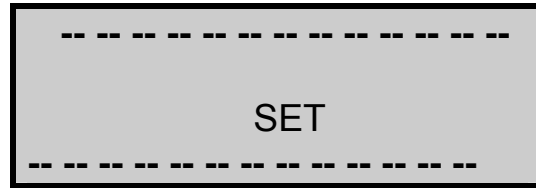Press the 



Pressing the  key displays



Parameter	Controls	Options
EFF	Select using  or  key and 	GROSS NET

6.4 Scale Options


The scale option routine gives you control over :-

- Language
- Line Rejection
- Gas Scale
- Compensation
- Temperature Scale
- Pressure Scale
- Reference Oxygen
- NOx calculation


TO SELECT SCALE OPTIONS




Press the  followed by 

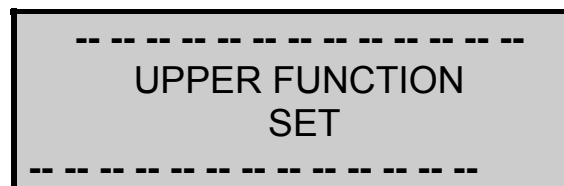UPPER FUNCTION key



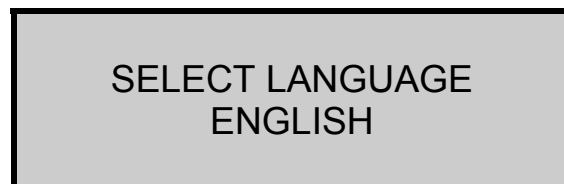


Pressing the  key displays






Parameter	Controls	Options
SELECT LANGUAGE	Select using  or  key and 	ENGLISH SPANISH NETHERLANDS FRENCH ITALIAN GERMAN SWEDISH FINNISH

SET LINE REJECTION
50 Hz

Parameter	Controls	Options
LINE REJECTION	Select using  or  key and 	50 Hz - UK 60 Hz - USA




ppm(n) or mg/m³(n)

Parameter	Controls	Options
GAS UNITS ppm(n) or mg/m ³ (n)	Select using  or  key and 	ppm ppm n mg/m³ mg/m³n




NOTE: ppm = parts per million
mg/m³ = milligrams per cubic meter
n denotes the reading is normalised or referenced to Oxygen
See Reference Oxygen in the Appendix

On power up the unit will default to ppm.




COMPENSATION < >
< OFF >

Parameter	Controls	Options
COMPENSATION	Select using  or  key and 	OFF ON

SET TEMPERATURE
CELSIUS




Parameter	Controls	Options
TEMPERATURE	Select using  or  key and 	CELSIUS FAHRENHEIT

SET PRESSURE
ppm

Parameter	Controls	Options
PRESSURE	Select using  or  key and 	mbar inWG

NOTE: mbar = millibar
 inWG = inches of water gauge

SET REFERENCE O2
NO

Parameter	Controls	Options
REFERENCE O2	Select using  or  key and 	NO YES

Selecting YES allows you to set an oxygen reference value different to that shown in the fuel constants. For example 3% is set in the Natural Gas constants, to reference the toxic gas values to a different value select using the screen below (Use the number setting sequence as detailed in Setting Time) :-

SET REFERENCE O2
REF. %O2 . . 03.0

This may need setting if a local authority require gas readings to be referenced to a certain oxygen value. As a general rule gaseous fuels are normally referenced to 3% oxygen.

NOTE: The readings can change dramatically if the wrong Oxygen reference is set and either ppmn or mg/m3n as the gas units. If you are unsure of the reference value set ppm or mg/m3 as detailed above.

SET NO_x CALC'N
NO

Allows the calculation for NO_x to be altered. Select YES to enter the following routine.

SET NO_x REF.
REF %NO_x. = 05

With only the NO sensor fitted there is no way of measuring NO₂ and an allowance is made in the calculation of the NO_x value. This NO_x value is calculated from the formula shown below :-




- $NO_x = NO + (P\% \times NO)$

where P% = REF. %NO_x and is set to 5% as default.

With both NO and NO₂ sensors fitted the formula is as follows :-

- $NO_x = NO + NO_2$

SET NO_x REF
NO_x = SUM

Parameter	Controls	Options
REF NOx	Select using  or  key and 	NOx = SUM NOx = NO NOx = NO2

There are three ways of displaying the value of NOx when the values are converted to mg/m3. Local authorities may require a certain calculation. The options are as follows:

- **NOx = SUM** calculates the mg/m3 figure individually from the NO and NO2 values and then adds them together.
- **NOx = NO** adds the ppm values together and then converts to NO equivalent.
- **NOx = NO2** adds the ppm values together and then converts to NO2 equivalent.

On power up the unit will default to NOx = SUM

6.5 Inlet Temperature

The Quintox uses as default the internal ambient sensor when calculating the Net temperature. If an optional inlet probe is fitted then INLET is used in the calculation.


As an alternative to both of the above, the inlet air entering the boiler can be measured using the flue probe.

NOTE: The probe must not be inserted into the flue until the INLET temperature has been set. If resetting the inlet temperature after performing a combustion test ensure the tip of the probe is at the air temperature


TO SET INLET TEMPERATURE

With the flue probe connected to the FLUE temperature connector.

Press the 

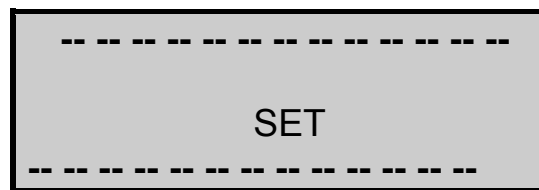


Pressing the  key displays

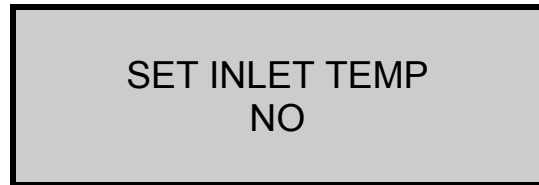


Change to YES

Position the tip of the flue probe near the Air inlet of the boiler and when the reading is stable press



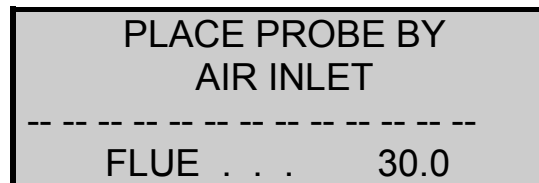

The temperature measured by the flue probe will be set in the Quintox.

Press  to check the reading.


6.6 Oxygen Calibration

If used over long periods the Oxygen sensor may drift slightly and for maximum accuracy may require resetting.


TO RESET OXYGEN SENSOR

With the flue probe sampling fresh air and the flue temperature reading less than 50°C/122°F, or the temperature plug disconnected from the instrument.


Press the

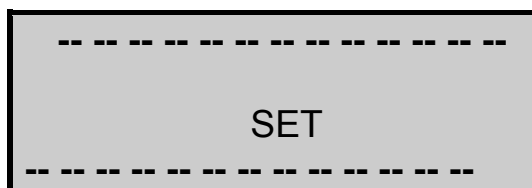

Pressing the



key displays

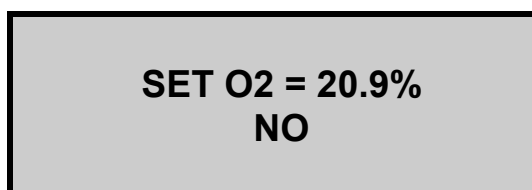

Change to YES

Press



to set 20.9% Oxygen.




6.7 Toxic sensor zero

The CO and other optional toxic sensors can be reset to zero if they drift. This may happen if the sensor is taken to very high concentrations for long periods of time or over-ranged.

Press




twice

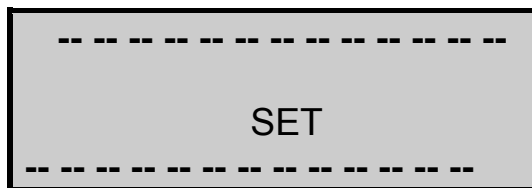




Press

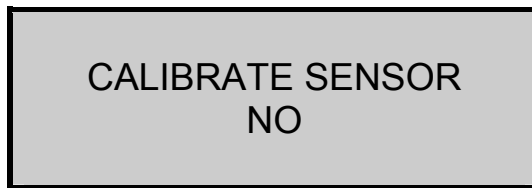


four times






Parameter	Controls	Options
-----------	----------	---------


CALIBRATE SENSOR	Select using  or  key and 	YES NO
-------------------------	--	-------------------------

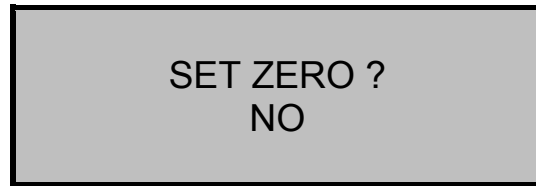


Select YES



Parameter	Controls	Options
SET ZERO	Select using  or  key and 	YES NO

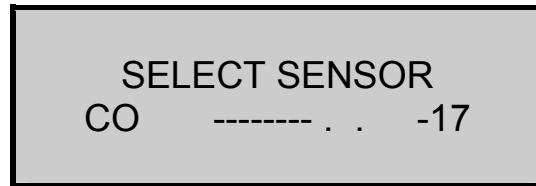Select YES




Parameter	Controls	Options
SELECT SENSOR	Select using  or  key and 	LIST OF FITTED SENSORS DISPLAYED

In this example we have selected the CO sensor. The pump will now run if it has been turned off, this is to draw **fresh air** through the instrument to allow the sensors to be zeroed.

Ignore the reading next to the sensor

Ensure the instability reads zero

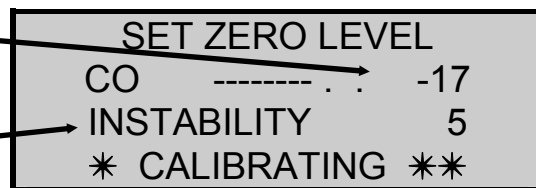

Once the instability has reached zero press



to accept the zero calibration and return to the main display.


If the instability does not reach zero then the instrument will show **FAULT**. Contact Kane International or Authorised Distributor for advice.

6.8 CO Alarm


It is possible to set a point in the range of the sensor so that it alarms and warns the user of a dangerous level of Carbon Monoxide. The default level is set at 400 ppm. This should be used when there is a local limit on the level of CO that should not be emitted from a boiler.

TO SET THE CO ALARM LEVEL


Press the

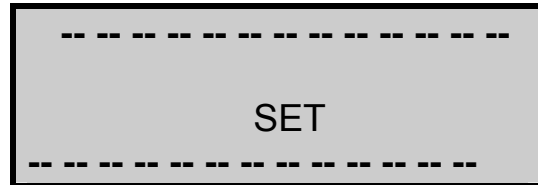

Pressing the




key displays

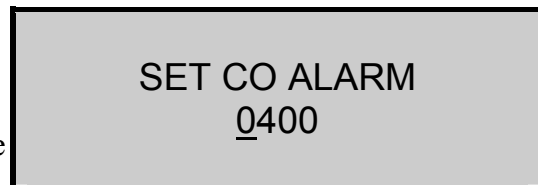

Set each number as detailed in Setting Time

When the CO level rises above the set value the following screen will be displayed every ten seconds. This will continue until the CO level falls below the alarm setting.

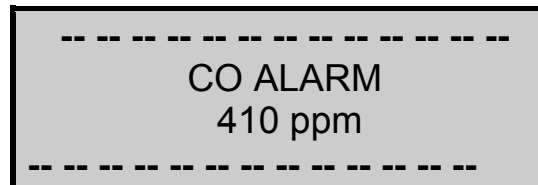

7. PRINTING INFORMATION

While in any of the main displays a manual print can be obtained by pressing

PRINT

The display will show the printout as it is printing :-

```
*** PRINTING ***
-----
** KANE-MAY **
-----
```

Standard Printout

The standard printout is shown below :-

```
-----
*** KANE-MAY ***
** KM QUINTOX **

DATE      02-01-97
TIME      18:14:35

      NATURAL GAS

O2  % ..... 20.9
CO  ppm ..... 0
Prs mbar    0.05
EFF %      FAULT

XAIR      O2 > 20%
CO2 % ..... 0.0
CO/CO2 R ... 0.0000
PI  % ..... 0.00

NO  ppm ..... 0
NO2 ppm ..... 0
NOx ppm ..... 0
SO2 ppm ..... 0
CxHy % ..... 0.0

NETT C ..... 0
FLUE C ..... 21
INLT  NOT FITTED
AMBIENT C 16.9

-----
```

The remainder of this section explains the following :-

Setting auto-timed printing or logging

Allows information to be printed or logged automatically at set time intervals (from 10 seconds to 90 minutes). Care must be taken in setting the interval time; a standard Quintox printout will take 30 seconds to print, it is advisable to set the interval at 2 minutes or greater if a print is requested. Turn off the printer if less than 2 minutes is set. If greater than 5 minutes is set the Quintox will switch OFF the pump immediately after printing and switch it ON again 3 minutes before the next print.

Disabling quintox printer

If only logged information is required without a printout then the Quintox integral printer can be turned OFF.

Edit the printout header

You can personalise the header on the printout to your own Company name and Telephone number. Two lines of 16 characters are available.


Changing the format of the printout

The standard printout is detailed on the previous page. You can customise a printout to your own requirements by selecting lines from the list detailed later in this section.

7.1 Changing printout parameters

Press  followed by  will display the following screens :


This displays the Auto print status and the interval time; for this example 2 minutes.

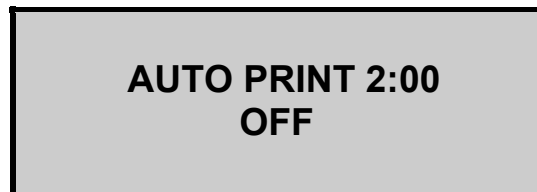




A rectangular display screen with a grey background and a black border. The text "AUTO PRINT 2:00" is centered on the top line, and "OFF" is centered on the bottom line.

Use  or  keys. To select ON or OFF and press 

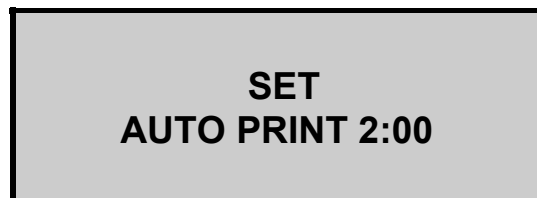With Auto print ON the display will show :-





A rectangular display screen with a grey background and a black border. The text "SET" is centered on the top line, and "AUTO PRINT 2:00" is centered on the bottom line.

Use  or  keys to select from 0:10 to 90:00 and press 

The next screen enables or disables the integral printer. Default is ON.



**PRINTER ?
ON**

Use  or  key to select **ON** or **OFF** and press

ENTER

To edit the printout header select **YES**.



**SET HEADER ?
NO**

Use  or  keys to select **YES** or **NO** and press

ENTER

The cursor will be positioned under the first *.

**EDIT HEADER
*** KANE-MAY ***
** KM QUINTOX **
ENTER & EFF=BACK**

Use  or  to select the alpha/numeric character required. Press **ENTER** when the character is correct. If you make a mistake the **EFF** key will take the cursor back.

ENTER

EFF

When the last character has been set the screen will display the next screen.

Entering NO will select the standard printout as detailed earlier in this section. The general principle for selecting a user printout is detailed below.

**USER PRINTOUT ?
NO**

7.2 User Defined Printouts

General Principle: A user defined printout can have a maximum of 40 lines. The contents of each line can be defined by the user from the master list of parameters detailed later in this section. The standard printout with line numbers and parameter numbers is given later in this section as an example. To define a printout you must allocate a parameter number to each line. The printout must be terminated with a line of hashes.



Select YES to configure your own printout.

```
USER PRINTOUT ?  
YES
```

```
SET LINE ..... ?  
NO
```

If you have previously configured a printout select **NO**, selecting **YES** will allow the first line of the printout to be changed.

```
SET LINE ..... 1  
* * KANE MAY * *
```

Use  or  keys to select the required line and press

```
ENTER
```

In this example the Time has been selected for the first line.

```
SET LINE ..... 1  
TIME                10:32:36
```

Repeat the process for the second line and so on.

```
SET LINE ..... 2  
O2 % .....        11.2
```

End the printout with a line of hashes.

```
SET LINE ..... 3  
#####
```

The above example will send the Time and Oxygen reading to the printout every two minutes.

To stop the Quintox Auto printing or logging, select Auto print **OFF** above and return to the main displays.

7.2.1 Standard Printout - Parameter Options Used:

LINE NUMBER	PARAMETER USED:	(MAX LINES: 40) & STATUS:
1	-----	PRINTOUT START
2		BLANK LINE
3	***KANE-MAY***	MANUFACTURER ID
4	**KM QUINTOX**	ANALYSER ID
5		BLANK LINE
6	DATE 02-01-97	DATE
7	TIME 18:14:35	TIME
8		BLANK LINE
9	NATURAL GAS	FUEL SELECTED
10		BLANK LINE
11	O2 %20.9	FLUE GAS O ₂ CONTENT
12	CO ppm0.0	FLUE GAS CO CONTENT
13	Prs mbar0.05	PRESSURE MEASUREMENT
14	EFF %.....FAULT	COMBUSTION EFF CALC
15		BLANK LINE
16	XAIR O2>20%	FLUE GAS EXCESS AIR
17	CO2 %.....0.0	FLUE GAS CO ₂ CALC (CO ₂ m% FLUE GAS CO ₂ MEASURE)
18	CO/CO2 R...0.00	CO/CO ₂ RATIO
19	PI %0.00	POISON INDEX
20	NO ppm.....0	FLUE GAS NO CONTENT
21	NO20	FLUE GAS NO ₂ CONTENT
22	NOx ppm.....0	NOX CALCULATION
23	SO2 ppm.....0.0	FLUE GAS SO ₂ CONTENT
24	CxHy % 0.0	HYDROCARBON READING
25		BLANK LINE
26	NETT C 0.0	NET FLUE GAS TEMP
27	FLUE C 21.0	ACTUAL FLUE GAS TEMP
28	INLT NOT FITTED	BOILER INLET TEMP
29	AMBIENT C 16.9	AMBIENT AIR TEMP
30	-----	DOTTED LINE

Not all parameters are used. See the master list on the next page if more are required.

7.2.2 Master List of Printed Parameters

The following list is a master list of printed parameters. Details of the measured and calculated variables are given in the Appendix.


	PRINT	DESCRIPTION
1	*** KANE-MAY ***	COMPANY IDENTIFICATION
2	** KM QUINTOX**	ANALYSER IDENTIFICATION
3	BLANK	BLANK LINE
4	DATE	DATE
5	TIME	TIME
6	INSTABILITY	FLUE GAS STABILITY STATUS
7	BATTERY	BATTERY STATUS
8	OS11	O ₂ SENSOR STATUS
9	SENSOR	SENSOR TEMPERATURE
10	AMBIENT	AMBIENT AIR TEMPERATURE
11	Prs	PRESSURE MEASUREMENT
12	NATURAL GAS	FUEL SELECTED
13	K1g	SELECTED FUEL GROSS CALORIFIC VALUE
14	K1n	SELECTED FUEL NET CALORIFIC VALUE
15	K2	SELECTED FUEL MAX THEORETICAL CO ₂
16	K3	SELECTED FUEL MAX WET LOSS
17	K4	SELECTED FUEL ALPHA VALUE
18	REF%O ₂	O ₂ REFERENCE - mg/m ³ n MEASUREMENTS
19	NETT	NET FLUE GAS TEMPERATURE
20	FLUE	ACTUAL FLUE GAS TEMPERATURE
21	INLT	BOILER AIR INLET TEMPERATURE
22	O ₂	FLUE GAS OXYGEN CONTENT
23	XAIR	EXCESS AIR CALCULATION
24	CO	FLUE GAS CO CONTENT
25	CO ₂	FLUE GAS CO ₂ CALCULATION (CO ₂ m FLUE GAS CO ₂ MEASUREMENT)
26	CO/CO ₂ R	CO DIVIDED BY CO ₂ RATIO
27	PI	POISON INDEX CO/CO ₂ RATIO X 100
28	EFF	COMBUSTION EFFICIENCY CALCULATION
29	LOSS	TOTAL LOSSES CALCULATION
30	DRY	HIGH TEMPERATURE & EXCESS AIR LOSSES
31	WET	LATENT HEAT LOSSES
32	CO LOSS %	INCOMPLETE COMBUSTION LOSSES
33	NO	FLUE GAS NO CONTENT
34	NO ₂	FLUE GAS NO ₂ CONTENT
35	NOX	FLUE GAS NOX CALCULATION
36	SO ₂	FLUE GAS SO ₂ CONTENT
37	CxHy	HYDROCARBON MEASUREMENT
38	H ₂ xc	CO/H ₂ CROSS SENSITIVITY MEASUREMENT
39	AUX1	AUXILIARY 1 SENSOR MEASUREMENT
40	-----	DOTTED LINE
41	#####	STOPS PRINTOUT

8. QUINTOX LOGGING AND PC DOWNLOAD

8.1 Overview


8.1.1 Description


Data is sent to the handset through the connection lead and can be stored if required. All information logged can be displayed on the hand-set, down-loaded to a computer or output directly to a printer.

The hand-set will store up to a maximum of 1926 pages (standard Quintox output). Information is stored each time the  key is manually pressed or an auto-timed print is requested.


The location number where the data is to be stored is displayed allowing it to be recorded on any paperwork e.g. job sheets.

8.1.2 Switching the Logger on

The logger can be operated either connected to the Quintox or as a standalone unit, (batteries are required if not connected). To turn the logger on use the  switch, the following will be shown on the display followed by the MENU screen.

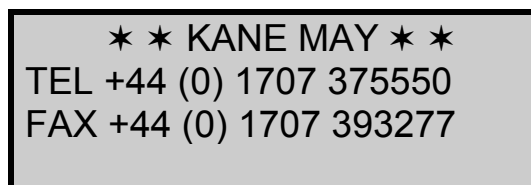

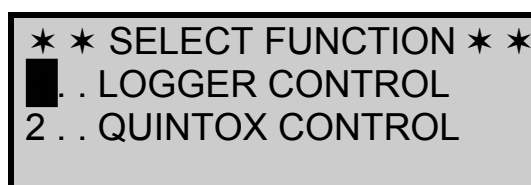

```
** KANE MAY **
TEL +44 (0) 1707 375550
FAX +44 (0) 1707 393277
```



```
** SELECT FUNCTION **
1 . . LOGGER CONTROL
2 . . QUINTOX CONTROL
```

LOGGER MENU


A flashing cursor will be positioned over the number **1**, control of the cursor is through and  and . Move the cursor to the desired function and press enter to select.

To return to the MENU at any time press  and  simultaneously.

8.1.3 Logging Data

Data logging is done with the handset operating in **2. QUINTOX CONTROL** and by either pressing the **PRINT** key or requesting an auto print, information will be captured by the logger and stored.

The display will show the following screen to confirm information has been stored correctly.

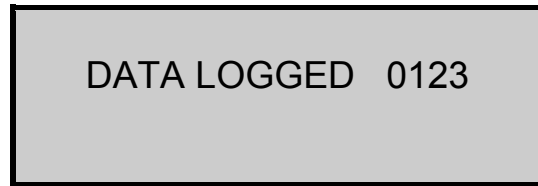

In the display shown above the data has been stored in location 123. Make a note of this on any paperwork you are using for that job so that the information can be retrieved later.

8.2 Batteries

The logging handset can either be powered from the Quintox through the lead or from its own batteries. Batteries are inserted in the back of the logger by removal of the rear cover.




TIP: It is advised that batteries are used at all times to ensure no data is lost or corrupted.

Four 'AA' alkaline batteries can be used or a Nicad rechargeable equivalent, if Nicad batteries are used they can be recharged by plugging the Quintox charger into the side of the handset. Typical recharge time is 12 hours.




Take care to insert batteries correctly, indication of polarity is in the battery enclosure.

8.3 Logger Control

This facility allows access to all of the information stored in the handset; data can be cleared, viewed on the display or output to a printer or PC. The logger records each page of Quintox information and gives it a unique log number; as additional logs are sent to the handset the log number is increased by 1 until a maximum of 1926 pages is reached. Once the memory is full, data will STOP logging.

To select **1. LOGGER CONTROL** position the cursor on the 1 in the MENU using  and  and press  . The first screen sets the language option,

SELECT LANGUAGE
ENGLISH




Parameter	Controls	Options
SELECT LANGUAGE	Use  and  to select the desired language, press  when correct	ENGLISH SPANISH NETHERLANDS FRENCH ITALIAN GERMAN SWEDISH FINNISH

CLEAR MEMORY
NO

Clear Memory allows you to clear all stored information prior to logging during tests, this resets the log number to **0001** so that the first new log is given this number.

Select **YES** or **NO** using  and  press  . A warning display is shown and you are requested to confirm you want to delete all of the data stored !

CONFIRM DELETION
YES

Select **YES** or **NO** using  and  press  .

LOG DATA ?
NO

ENTER YES to tell the logger to store data in memory and **NO** to disable the logging function.

DOWNLOAD MEMORY
NO

Download Memory allows you to output the stored information to a PC, output is in our own format and requires a special program to extract the data. Contact Kane International or Distributor for information on the 'Fireworks' range of software.

Selecting **YES** will set the handset in **READY** mode, this allows the PC software to access the data stored.

READY

Once the PC has extracted the data from the handset the logger will revert back to the **LOGGER MENU**.

WARNING ! The logger will stay in **READY** mode until all of the data is extracted from the handset. Do not enter this mode unless you are going to download data - you will have to switch **OFF** the handset if you do.

DISPLAY MEMORY
NO




Display Memory allows you to view stored information on the hand-set display.

Select YES to access the following screen.


DISPLAY MEMORY
SELECT 0000 TO 0123
0000

ENTER the desired location to display the memory **FROM**. Entering numbers is detailed in section 6.



LOG NO.	0100
DATE	23/10/96
TIME	10:32:36
BATTERY %	54

To scroll through data, use  and , note the log starts with the Log Number followed by Quintox data. Note also that once at the top of a log the  will take you to the top of the previous log i.e.

LOG NO.	0099
DATE	23/10/96
TIME	10:31:36
BATTERY %	54

Using the  will scroll through that particular log moving one line at a time.

DATE	23/10/96
TIME	10:31:36
BATTERY %	54
INSTABILITY	1

To exit Display Memory, press  and  together and return to the **LOGGER DISPLAY**.

8.4 Downloading Information

Data can either be downloaded from the handset or stored directly in a PC realtime. To extract the data from the handset contact Kane International for information of the FIREWORKS range of software. The software allows information to be extracted from the handset or gather information from the PC.


Other features of the FIREWORKS software are :-

- Graph and print stored and realtime data.
- Display information on bar graphs and large LED type display.
- Compile tuning reports and emissions reports.
- View data stored in tabular format.
- Export files to spreadsheet format.
- Allow the PC to act as a virtual handset and control the Quintox.

Stored data can not be extracted from the handset without the FIREWORKS software. Information can be captured from the RS232 on the Quintox. A standard RS232 serial lead is required to connect the Quintox RS232 to the PC serial port. Contact your computer supplier or Kane International for the required lead. Leads are supplied with the FIREWORKS software.

8.4.1 Setting Up Your PC

A standard communications package will be able to collect the data from the Quintox. Windows Terminal software is a suitable package. The communications protocol should be set to :-

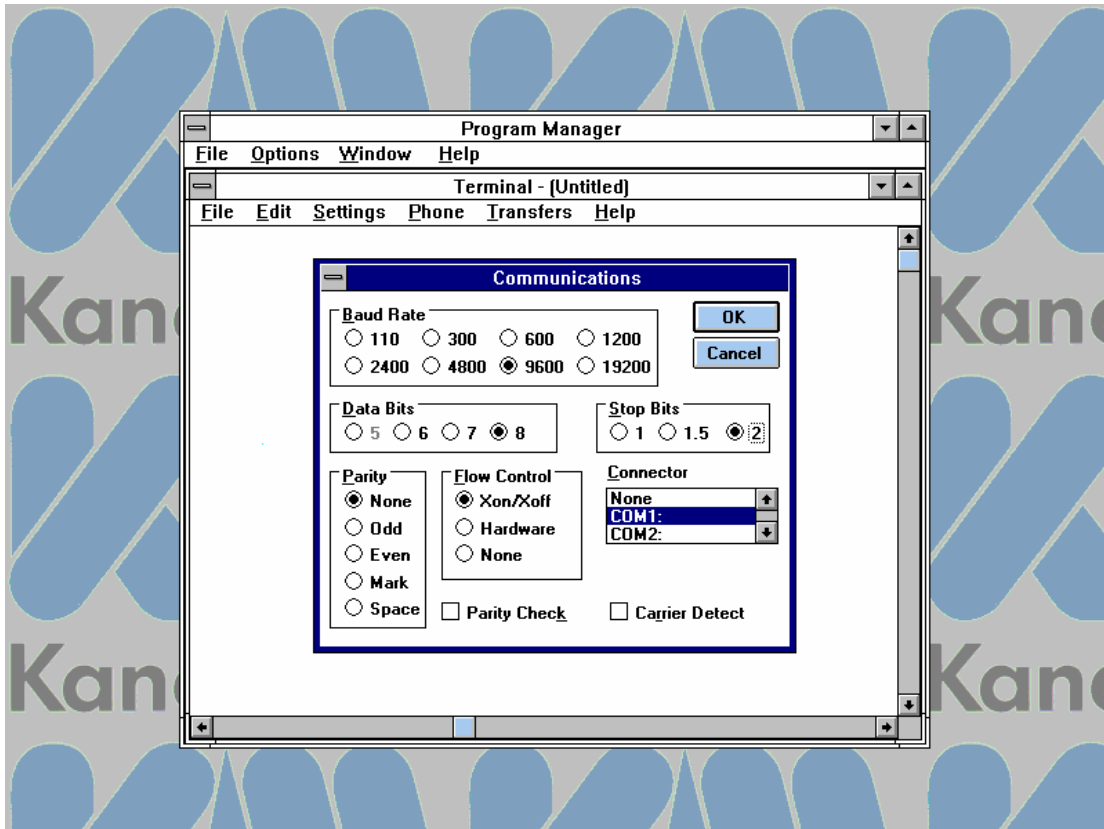

8.4.2 Capturing Data From Quintox

To capture data direct from the Quintox into a PC the RS232 port on the Quintox has to be connected to the serial port on your PC. Using the standard RS232 lead, and IBM/AT lead if your serial port is a 9 pin D type, connect the Quintox to the PC.

The RS232 can output in two formats, Comma Separated variable (CSV) and Binary (for the logger).

The standard default setting is binary and will always be set if the instrument is switched off and on. To change between the outputs press



followed by



The instrument will beep and change the output, repeat the key sequence to change back. The format for the CSV output is as follows:-

Time	Date	Instability	Battery	Sensor	Ambient	Pressure	Fuel
16:28:30	20-05-96	0	49	23.5	24.5	0.3	12

K1g	K1n	K2	K3	K4	O2 Reference	Nett temp	Flue temp
0.35	0.39	11.8	9.8	32	3	120	144

Inlet temp	Oxygen reading	Excess air	CO Reading	Calculation	Efficiency	Losses	Dry loss
N	8.3	28	55	3.5	83	17	8

Wet loss	CO Loss	NO	NO2	NOx	SO2	H2xc	Aux1	Aux2
7	2	20	N	21	N	12	N	N

The output will be as the example below:-

16:28:30, 20-05-96, 0, 49, 23.5, 24.5, 0.3, 12, 0.35, 0.39, 11.8, 9.8, 32, 3, 120, 144, N, 8.3, 28, 55, 3.5, 83, 17, 8, 7, 2, 20, N, 21, N, 212, N, N

Where a number is not displayed the following meanings can be taken:-

N = Not fitted

F = Fault

O = Over range (i.e. Oxygen reading 20.9% hence excess air can not be calculated)

8.4.3 Downloading Logged Data

The FIREWORKS software allows data to be downloaded from the handset. This section is supplied to explain how to set the handset in a state ready to transmit data.

Using the lead RE5PC supplied with FIREWORKS connect the 15 pin D connector to the handset and the 9 pin D connector to your PC serial port. Most PCs have a 9 pin D serial port if yours has a 25 pin contact your computer supplier for a convertor.

Set the logger to **DOWNLOAD** data and ensure it is in **READY** mode.

NOTE: You will require batteries to run the logger and download the data.

9. CONTINUOUS MONITORING

The Quintox is designed primarily as a portable emissions monitoring analyser. It can however be used for longer periods if the gas is treated correctly before being supplied to the analyser.

The main problem with continuous monitoring is the build-up of water in the water trap. There are two methods available for extracting the water. Both are optional extras available :-

- Pump drained water trap with built-in level sensor. This connects via RS232 connections and will automatically drain the water trap if the level rises too high. The electronics in the water trap will also stop the Quintox from pumping if the water level does not drop.

Gas Conditioning Unit with heated line and cooled chamber. This should be used when accurate NO₂ and SO₂ readings are required. A Main Purge solenoid should also be fitted to the Quintox when monitoring for longer periods of time. This is to supply fresh air to the sensors and hence prevent them drying out. See Recommended Operation in next section.

10. Main Purge

The main purge facility for Quintox is used where longer sampling of flue gas is required. It should be used with the KM9008 gas conditioning unit or in conjunction with any other water removal system.

If dry gas is supplied to the Quintox for a long period of time the operating cells will dry out and stop working. Supplying fresh ambient air to the sensors on a periodic basis will prevent or reduce the drying effect and prolong sensor life. Ideally the fresh air should be at 50% relative humidity but it is understood under certain conditions this may not be possible.

Main purge introduces a solenoid valve into the gas train after the water trap connection to the Quintox. With the purge turned OFF the instrument will draw gas from the probe and flue, with purge ON the solenoid is activated and the instrument draws fresh air from within its case. The solenoid can be switched either manually or through a timed operation.

Manual Operation

This function allows the user to switch the solenoid ON or OFF manually through pressing a sequence of keys. It can be performed at any time during Quintox operation but has no effect during a timed operation.

ON/OFF Toggle operation



Timed Operation

This requires the user to set the following :-

Purge duration - The amount of time fresh air is draw into the instrument. This can be set between 5 and 30 minutes and is a function of the gas concentration and the humidity of the ambient air. For dry ambient conditions and high gas concentrations a longer purge duration should be set.

Purge interval - This is the time between purge operation, i.e. the time the instrument is sampling gas. It can be set between 9 and 99 minutes.

Auto zero - Allows all toxic cells to be set to zero and the oxygen cell to 20.9% on completion of the purge cycle. i.e. if 10 minutes is set in the 'Purge duration' following this time the cells would be Auto zeroed. Note sufficient time must be allowed for the cells to return to zero, if concentrations of gas are high then a long purge duration should be set.

NOTE: If the analyser is positioned where levels of gases are higher than fresh air ambient conditions then auto zero should not be used.

To access timed purge enter the following :-

SET/CAL
ENTER

SET/CAL
ENTER

Enter the code 0000 at the following display :-

ENTER SERVICE CODE
----- > 0 0 0 0 < -----

The following screens will be displayed, enter NO to both :-

CALIBRATE SENSOR
NO

PRINT MEMORY ?
NO

The purge sequence now begins, by using the arrow keys select YES to 'SET PURGE ?' and press

ENTER

SET PURGE ?
YES

Enter the purge duration and similarly the purge interval by changing each character. Note the line below the zero indicates the number to be changed. Enter when correct. If a time of less than the minimum or greater than the maximum then these will set as the default values.


PURGE DURATION 05
<05 09>

PURGE INTERVAL 30
<09 99>

Set YES or NO depending on whether auto zero is required or not.



Note: During both Manual and Timed purge operation the following screen will be displayed for approximately one second every 3 seconds.

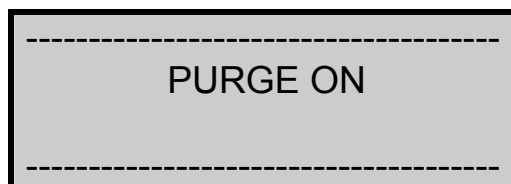

Recommended Operation

Each monitoring situation will be different and a degree of user judgement will apply. The following basic guidelines should be followed :-

- Maximum duration without purge 4 hours followed by 40 minutes purge.
- For monitoring up to 12 hours per day purge should be for 10 minutes every hour.
- For monitoring up to and over 24 hours per day purge should be for 10 minutes every 30 minutes. This could be a sequence of 5 minutes purge followed by 10 minutes sample.

Sensor Over-range


The main purge will also operate when any gas concentration goes over the stated range of that sensor. Fresh air will be drawn into the Quintox until the gas level is down to 80% of the sensor range.

11. MAINTENANCE

11.1 Emptying and Cleaning the In-line Water Trap

The water trap should be checked and emptied on a regular basis. Water vapour will condense and gather in the probe line this may move suddenly to the trap when the probe is moved. Care should be taken at all time.


Emptying of the water trap is detailed below :-

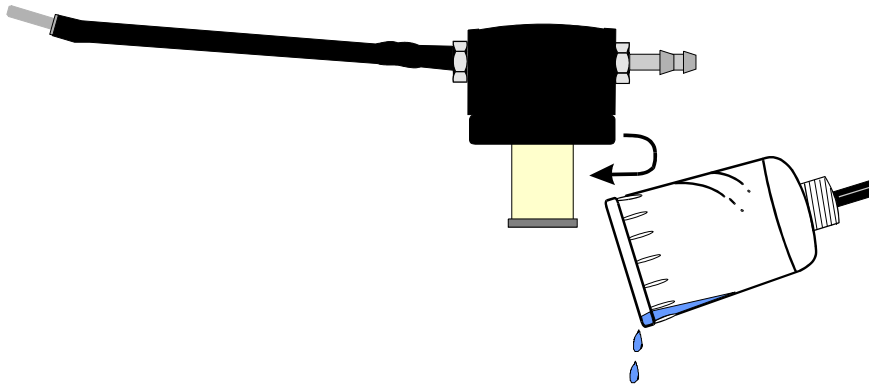

Carefully remove the end cap from the in-line housing. Dispose of the condensate in a suitable drain, care must be taken as it could be acidic. If condensate spills onto the skin or clothing, clean off immediately using fresh water, seek medical advice if problems occur.

11.2 Changing the Particle Filter

This is a very important part of the analyser and should be changed regularly. It prevents dust and dirty particles entering the pump and sensors and hence causing damage. The filter **MUST** be changed when it appears discoloured.

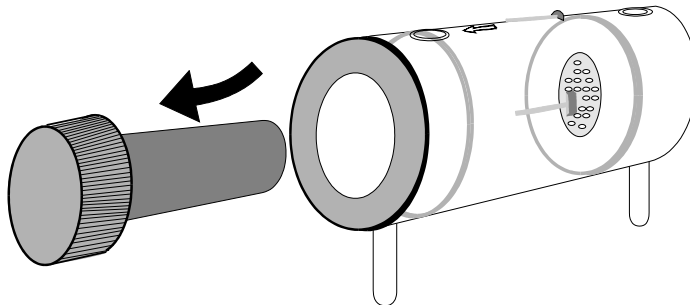

Remove the end cap from the filter housing. Carefully remove the paper filter element and dispose of it. Clean the inside of the filter housing with a suitable soft cloth. Insert a new filter element onto the spigot on the filter end cap and carefully insert it into the filter body.

11.3 Charging the Battery

It is important that the battery is charged on a regular basis. The instrument constantly powers the internal sensors and may flatten the battery if left unattended for some months. Connect the charger supplied with the instrument to the correct mains supply.


Note: The correct charger type is required for your local voltage i.e. 110 or 220 volts AC

Insert the plug in the socket marked CHARGER INPUT SOCKET as detailed in section 1.4.

The CHARGER ON GREEN LED will illuminate showing the instrument is charging.

11.4 Changing the Paper Roll

To change the paper roll remove the printer cover by loosening the two screws holding it down. Remove the old paper roll core and insert the new roll so that it sits as follows :-

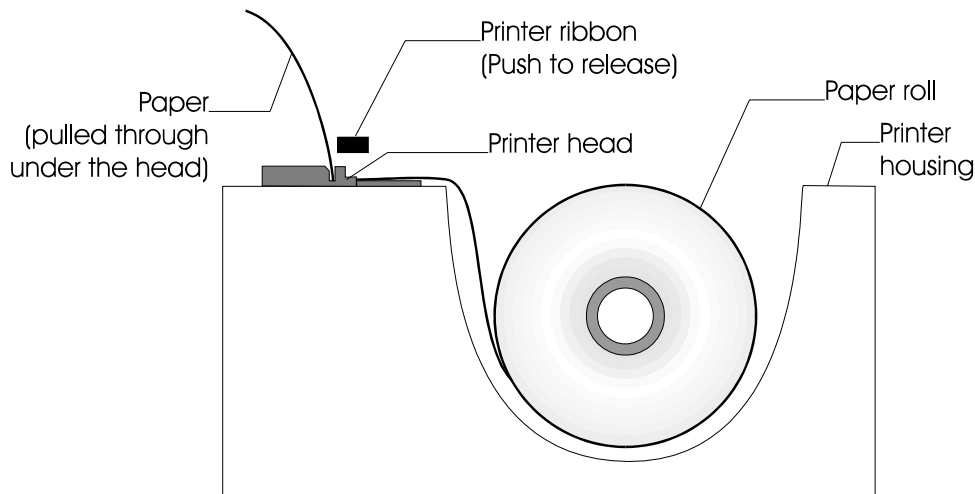

Feed the free end of paper into the printer through the metal slot beneath the printer ribbon. Start the paper feed sequence until the paper has emerged from the top of the printer, feed the loose end through the cover and refit.

TO START PAPER FEED

Press the **SET/CAL** followed by




UPPER FUNCTION key



Pressing the **PRINT** key displays



Press any key to stop.

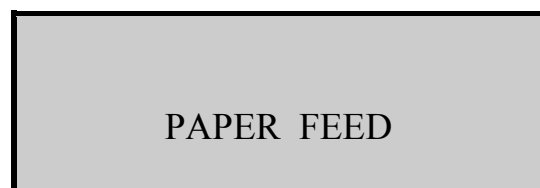


11.5 Changing the Printer Ribbon

The printer ribbon cartridge will last for approximately two rolls of paper. Remove the printer cover as detailed above.

Marked on one end of the cartridge is PUSH. Gently press down on this end and the ribbon cartridge will pop up at the other end. Remove the cartridge and dispose of.

Fit a new ribbon guiding the paper roll between the exposed ribbon and cartridge body.

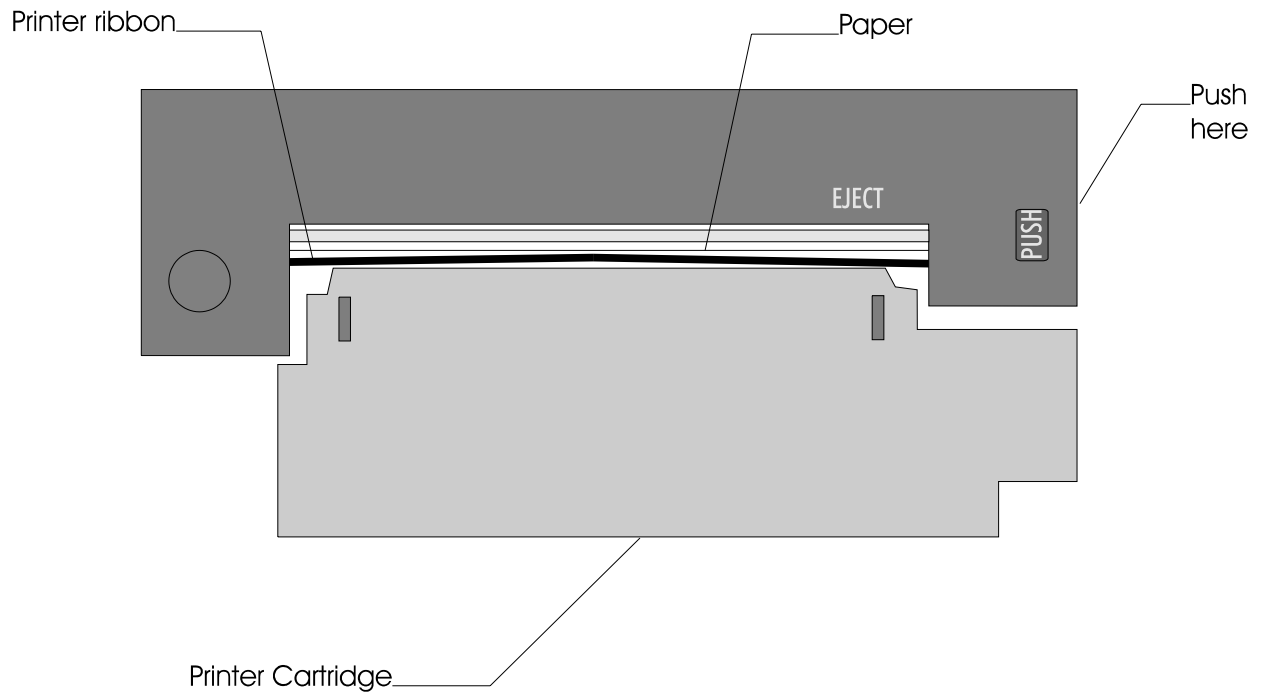

Refit printer cover.

12. PROBLEM SOLVING

The following is a list of problems that may occur on the instrument through its operating life. If the cause of the fault is not easy to identify then we advise you to contact the Kane International Service Department or an International Distributor for expert advice.

Fault symptom	Causes
<ul style="list-style-type: none"> • Oxygen too high • CO₂ too low 	<ul style="list-style-type: none"> • Air leaking into probe, tubing, water trap, connectors or internal to instrument. • Oxygen cell needs replacing.
<ul style="list-style-type: none"> • Oxygen Error (FAULT) • Toxic sensor Error (FAULT) 	<ul style="list-style-type: none"> • Calibration time set too short and instrument not allowed to stabilise • Instrument has been stored in a cold environment and is not at normal working temperature. • Oxygen cell or toxic sensors needs replacing.
<ul style="list-style-type: none"> • Analyser not holding charge • Analyser not charging 	<ul style="list-style-type: none"> • Battery exhausted. • AC charger not giving correct output. • Fuse blown in charger plug.
<ul style="list-style-type: none"> • Analyser does not respond to flue gas 	<ul style="list-style-type: none"> • Particle filter blocked. • Probe or tubing blocked. • Pump not working or damaged with contaminants. • Probe connected to pressure connector.
<ul style="list-style-type: none"> • Flue temperature readings erratic 	<ul style="list-style-type: none"> • Temperature plug reversed in socket. • Faulty connection or break in cable or plug.
<ul style="list-style-type: none"> • Analyser automatically switches off in operation. 	<ul style="list-style-type: none"> • Battery below alarm level. • Battery quickly discharging and is faulty.
<ul style="list-style-type: none"> • Display is blank. 	<ul style="list-style-type: none"> • The contrast setting has been lost and requires resetting. Disconnect handset lead and reconnect. Set contrast as in Section 5.4

13. ANNUAL RE-CALIBRATION


Whilst the sensors have an expected life of more than two years in normal use it is recommended that the analyser is re-calibrated at least annually. This is so that long term drift on the sensors and electronics can be eliminated. Local regulation may require more frequent re-calibration and users should check with appropriate authorities to ensure they comply with relevant guidelines.

14. HOW TO GET EXPERT HELP


There will be occasions when despite having read the manual there will be problems that you cannot resolve and so you need external help.

Before calling Kane International or one of its International Distributors please first check the following:


Find the serial number of the instrument. It is located on the label close to where the charger and handset leads plug into the analyser. Also make a note of which sensor are fitted by observing the tick boxes on the same label.

If the handset and analyser are operating you can also determine the issue of software loaded in the analyser. To find this complete the start-up calibration routine and the press  twice .

The display will show


Use the  key to change the numbers

```
ENTER SERVICE CODE
-----> 0 0 0 0 <-----
```

Then press  to step to the next number

You need to enter

```
ENTER SERVICE CODE
-----> 1 1 1 1 <-----
```

Press  again and the display will show

```
Issue 15.0 . . . . . G
- 1 2 3 4 5
```

Please record the issue number.

Press any key to exit this mode.

When you call the relevant Service Dept please have this information available so that the technician has the best chance of being able to help you. If you have a modem you may be asked to connect the RS232 interface of the analyser to your modem so that the technician can operate the analyser remotely and extract from it information stored in its memory that might help to resolve your problem.

15. PRODUCT SPECIFICATION

INSTRUMENT

Parameter	Resolution	Accuracy	Range
Temp Measurement			
Flue Temperature	0.1° (C/F)	1.0° C +/-0.3% of reading	0 - 1100°C, 32 - 2140°F * Use high temperature probe for gases > 600°C/1112°F
Inlet Temperature	0.1° (C/F)	1.0° C +/-0.3% of reading	0 - 600°C 0-999°F
Gas Measurement			
Oxygen (O ₂):	0.1%	-0.1% +0.2%	0-25%
Carbon Monoxide (CO):	1ppm	+/-20ppm < 400ppm 5% of reading < 2000ppm +/- 10% of reading	0 - 10,000ppm
Carbon Monoxide (CO):	0.01%	>2000ppm +/- 5% of reading from	0 - 10%
Nitric Oxide (NO):	1ppm	0.1% to 10% +/- 5ppm < 100ppm	0 - 5,000ppm
Nitrogen Dioxide (NO ₂):	5ppm	+/-5% of reading >100ppm +/-5ppm < 100ppm	0 - 1,000ppm
NitrogenOxide (NO) ^H :	1ppm	+/-5ppm < 500ppm +/-5% of reading >	0 - 5,000pm
Pressure:	0.01mbar/kpa	500ppm +/-5% of reading >100ppm	0 - 150mbar
Sulphur Dioxide (SO ₂):	0.1%	+/-0.5% Full scale	0 - Fuel Value
Carbon Dioxide (CO ₂)	0.1%	+/-7% of reading +/-0.4%	0-100%
Carbon Dioxide (CO ₂) ^{*2} :	0.01%	+/-0.3%	+/-5% of reading
Efficiency ^{*2} :		+/-1%	
Hydrocarbons (HC):		0-5% Methane (LEL)	

*1 Using dry gases at STP

*2 Calculated

LEL = Lower Explosive Limit

HANDSET

Dimensions	220 mm long 120 mm high 50 mm wide
Keypad	16 tactile keys with sounder
Display	4 line LCD with backlight and contrast control

EXTENSION CABLE

Specification:	8 pin DIN to 15 pin 'D' screened cable
Cable lengths:	5m Standard 10-20m-Optional

PROBE

Choose from a range of probe options. See probe leaflet.

BATTERY

Type:	Lead acid rechargeable (12V, 2 AH)
Life:	8 hours from full charge
Charge time:	12 hours

BATTERY CHARGER

Input:	110-120V AC/220-240V AC.
Output:	16V AC (RMS)@ 1 amp, 50-60 hz.

PUMP

Flow rate:	2 Litres/Minute nominal
------------	-------------------------

PRINTER

16 character dot matrix.

RS232

25 way plug connector,
9600 Baud,
No parity,
8 Data bits,
2 Stop bits.

QUINTOX	PC
Pin 2: TXD	Pin 2: TXD
Pin 3: RXD	Pin 3: RXD
Pin 4: RTS	Pin 4: RTS
Pin 5: CTS	Pin 5: CTS
Pin 7: Ground	Pin 7: Ground

AMBIENT OPERATING RANGE

0 - 40°C (+32°F to 104°F)

20 - 80% RH non condensing

Storage: 0-50°C

Maximum gas temperature at sensors:

Continuous +40°C

Intermittent +55°C

APPENDICES

A - Parameter Meanings

The parameters and their meanings are detailed as follows : -

- DATE :** Analyser date. See Section 6.1 to change.
- TIME :** Analyser time. Use Section 6.1 to change.
- INSTABILITY :** This is an indication of how stable the signals are from all the sensors. 0 = high stability, 10 = high instability. When measuring flue gases, pressure and temperature this number will rise as the sensed inputs varies. At start up when sampling fresh air this number is invariably 0.
- BATTERY :** Displays the battery level from 0-100%. The analyser will flash **RECHARGE BATTERY** at less than 10 % of charge. The analyser may show levels greater than 100% when the charger connected.
- FUEL :** The fuel used in calculation of efficiency and Carbon Dioxide.
- K1g:** Gross calorific fuel constant. See Appendix B for calculation.
- K1n :** Gross calorific fuel constant. See Appendix B for calculation.
- K2 :** Percentage Maximum theoretical CO₂ (dry basis).
- K3:** Percentage wet loss.
- K4 :** Percentage unburnt carbon loss.
- O2r :** Toxic gas measurements can be referenced to defined oxygen levels.

Oxygen referencing is required by some regulations such as TA-LUFT. If a reference value is selected the toxic gas measurements will be displayed with the symbol **n** attached to the units. i.e.ppmn

What does Oxygen reference mean ?

If 3 % O₂ reference is selected and 5 % O₂ is measured in the flue then toxic gas values will be recalculated as if 3 % were measured. The equation for referencing is detailed in the Appendix.

Oxygen referencing prevents false readings being submitted, e.g. allowing more air into the boiler will increase the oxygen level in the flue and hence dilute any toxic gas reading. Oxygen referencing gives readings as if they were undiluted.

- NETT :** Nett temperature calculated by deducting the internal AMBIENT temperature from the measured FLUE temperature. Displays in either Centigrade C or Fahrenheit F and will display NOT FITTED if flue probe not connected.
- If an external INLET probe is used then INLET is deducted from FLUE.
- O2 :** Oxygen reading in percentage %.
- CO :** Carbon Monoxide reading indicated in ppm or mg/m³. If the figures are referenced to oxygen then the display will show **ppmn** or **mg/m³n**. See Section 6.4 for oxygen reference. Note with a high CO sensor fitted the reading will be displayed in percentage %.
- EFF (G) :** Combustion Efficiency calculation displayed in percentage. Gross G or Net N can be set see Section 6.3. The calculation is determined by fuel type see Appendix B for calculation. The efficiency is displayed during a combustion test, 00.0 is displayed while in fresh air.
- CO2m:** Carbon Dioxide reading in percentage %
- CO2 :** Carbon Dioxide calculation determined by the type of fuel. This only shows a reading when a combustion test is being carried out. Zero (0.0) is displayed while in fresh air.
- FLUE :** Temperature measured by flue gas probe in Centigrade or Fahrenheit. Will show ambient temperature after fresh air calibration and **NOT FITTED** or **FAULT** if probe disconnected.
- INLET :** Temperature measured by the optional inlet air probe or stored using the Flue probe See Section 6.5. The air probe is plugged into the instrument through the INLET socket. This figure is used to calculate the NET temperature instead of AMBIENT when fitted.
- AMBIENT :** Temperature measured by the internal sensor, used in the NET temperature

CO/CO₂ R : The CO/CO₂ ratio, is the ratio of measured CO divided by CO₂.

It gives an indication of the following :-

- How good a gas sample the instrument is reading.
- How clean the boiler is running.

For example : A new or clean domestic boiler will display a ratio of less than 0.004, a unit in need of cleaning 0.004-0.008 and a unit in need of major overhaul will show greater than 0.008.

This only shows a reading when a combustion test is being carried out. 0.0000 is displayed while in fresh air.

P INDEX : The CO/CO₂ ratio expressed as a percentage %, called the 'Poison Index'
i.e. P INDEX % = 100 x CO/CO₂. 0.00 is displayed while in fresh air.

XAIR % : Excess air calculated from the measured oxygen and type of fuel used.
Displays reading during a combustion test. O₂ > 20% is displayed while in fresh air.

Prs : Flue draught pressure reading. Displayed when pressure sensor fitted. See section 4.5 for taking a reading and Section 6.4 for changing for scale.

NO: Nitric Oxide reading in ppm or mg/m³. Displayed when Nitric Oxide sensor fitted. Reading can also be referenced to oxygen ppmn or mg/m³n.

NO₂: Nitrogen Dioxide reading in ppm or mg/m³. Displayed when Nitrogen Dioxide sensor fitted. Reading can also be referenced to oxygen ppmn or mg/m³n.

NO_x : Calculated total Nitric oxides displayed in ppm or mg/m³.
For more details on NO_x calculation see Section 6.4 Scales.
Reading can also be referenced to oxygen ppmn or mg/m³n.

SO₂ : Sulphur Dioxide reading in ppm or mg/m³. Displayed when Sulphur Dioxide sensor fitted. Reading can also be referenced to oxygen ppmn or mg/m³n.

- CxHy :** Unburnt HydroCarbon reading in % of LEL of Methane, the sensor is calibrated with Methane. Displayed when a HydroCarbon sensor fitted.
- LEL is the Lower Explosive Limit of a gas when mixed with air, for Methane this has the ratio of 19:1 Air:Methane. Below the LEL the mixture can not ignite and burn. In the Flue unburnt HydroCarbons should be well below this level or there is the potential for an explosion.
- LOSS :** Total losses calculated from Combustion Theory. This is the summation of the next three parameters.
- DRY :** Calculated heat lost in turning the Carbon in the fuel to Carbon Dioxide (CO₂).
- WET :** Calculated heat lost in turning the Hydrogen in the fuel into water (H₂O).
- CO LOSS % :** Calculated loss due to partially burnt Carbon. Any Carbon Monoxide (CO) in the flue has the potential to be turned into Carbon Dioxide and release more heat, hence this heat is lost up the flue.
- OS11 % :** Oxygen sensor life indicator. This is an approximation calculated from the output voltage of the sensor in **fresh air**. Note ! This is not valid when a combustion test is being performed.
- H2xc :** The Carbon Monoxide sensor is Hydrogen compensated. This parameter is the reading from the Hydrogen sensor built into CO sensor. It is an indication of the level of Hydrogen in the flue and can NOT be used as an exact level, it is only used to cross compensate the CO sensor.
- AUX1 :** Auxilliary sensor position, to be used for future sensors.

B. NO_x CALCULATIONS

ONLY an NO Sensor fitted.

working in ppm: NO_x referenced to NO

The user can select the **assumed NO₂ percentage** and the **O₂ normalised** level

then: $NOx \text{ in ppm} = NO \text{ in ppm multiplied by } (1 + \text{assumed } NO_2 \text{ percentage})$

in this setup NO_x can only be displayed as NO_x = NO

then normalising:

$NO \text{ in ppmn} = NO \text{ in ppm multiplied by } (21 \text{ minus the } O_{2norm} \text{ setting})$
and then divided by (21 minus the actual O₂ reading)

For a worked example assume:

NO is 1000ppm

NO₂ is 5% of NO

O_{2norm} is set to 3%

actual O₂ is zero

$$NOx \text{ in ppm} = 1000 \times (1 + 5/100) = 1000 \times 1.05 = \mathbf{1050} \text{ ppm}$$

$$NO \text{ ppm n} = 1000 \times (21 - 3)/(21 - 0) = 1000 \times 18 / 21 = \mathbf{857} \text{ ppm n}$$

$$NOx \text{ ppm n} = \mathbf{1050} \times 18 / 21 = 900 \text{ ppm n}$$

or

$$NOx \text{ ppm n} = \mathbf{857} \times 1.05 = 900 \text{ ppm n}$$

working in mg/m³: NO_x referenced to NO or NO₂

The user can select the assumed NO₂ percentage, the O₂ reference level and whether the NO_x reading is referenced to NO or NO₂

referenced to NO

$NO \text{ in mg/m}^3 = NO \text{ in ppm multiplied by } 1.34$

$NOx \text{ in mg/m}^3 = NO \text{ in mg/m}^3 \text{ multiplied by } (1 + \text{assumed } NO_2 \text{ percentage})$

NOx referenced to NO₂

NOx in mg/m³ = NO in ppm multiplied by 2.05 multiplied by (1 + assumed NO₂ percentage)

or

NOx in mg/m³ = NO in mg/m³ divided by 1.34, multiplied by 2.05 and multiplied by (1 + assumed NO₂ percentage)

normalising readings

normalised reading = initial reading multiplied by (21 minus the O_{2norm} setting) and then divided by (21 minus the actual O₂ reading)

BOTH NO and NO₂ sensors Fitted

Working in ppm $NO_x = NO + NO_2$

normalising readings

ppm = initial reading in ppm multiplied by (21 minus the O_{2norm} setting) and then divided by (21 minus the actual O₂ reading)

Working in mg/m³

The user can select how the readings are referenced.

NO_x = SUM
NO_x = NO
NO_x = NO₂

NO_x = SUM

NOx in mg/m³ = NO in ppm multiplied by 1.34 plus NO₂ in ppm multiplied by 2.05

NO_x = NO

NOx in mg/m³ = (NO in ppm plus NO₂ in ppm) multiplied by 1.34

NO_x = NO₂

NOx in mg/m³ = (NO in ppm plus NO₂ in ppm) multiplied by 2.05

normalising readings

ppm = initial reading in ppm multiplied by (21 minus the O_{2norm} setting) and then divided by (21 minus the actual O₂ reading)

mg/m³ = initial reading in mg/m³ multiplied by (21 minus the O_{2norm} setting) and then divided by (21 minus the actual O₂ reading)

ONLY an NO₂ sensor fitted

When there is only an NO₂ sensor fitted the NO_x function is disabled

$$NO_2 \text{ in } mg/m^3 = NO_2 \text{ in ppm multiplied by } 2.05$$

normalising readings

ppm_n = initial reading in ppm multiplied by (21 minus the O_{2norm} setting) and then divided by (21 minus the actual O₂ reading)

mg/m³_n = initial reading in mg/m³ multiplied by (21 minus the O_{2norm} setting) and then divided by (21 minus the actual O₂ reading)

C. COMBUSTION EFFICIENCY CALCULATION

The efficiency calculation is based upon British Standard BS845.

This identifies three sources of loss associated with fuel burning:

Losses due to flue gasses: Dry Flue gas loss,
Moisture and hydrogen
Sensible heat of water vapour
Unburned gas

Losses due to refuse: Combustible in ash
Combustible in riddlings
Combustible in dust

Other losses: radiation
convection
conduction
other unmeasured losses

Net efficiency calculations assume that the energy contained in the water vapour (formed as a product of combustion and from wet fuel) is recovered and the wet loss term is zero. Gross efficiency calculations assume that the energy contained in the water vapour is not recovered.

Since the fuel air mixture is never consistent there is the possibility of unburned/partially unburned fuel passing through the flue. This is represented by the unburned carbon loss.

Losses due to combustible matter in ashes, riddlings, dust and grit, radiation, convection and conduction are not included.

Efficiency Calculation:

Known Data - Fuel: Q_{gr} = Gross Calorific Value (kJ/kg)
 Q_{net} = Net Calorific Value (kJ/kg)
 $K1$ = Constant based on Gross or Net Calorific Value:
 $K1g = (255 \times \% \text{Carbon in fuel}) / Q_{gr}$
 $K1n = (255 \times \% \text{Carbon in fuel}) / Q_{net}$
 $K2$ = % max theoretical CO_2 (dry basis)
 $K3$ = % Wet Loss

Measured Data: T_f = Flue Temperature
 T_i = Inlet Temperature
 O_{2m} = % Oxygen in flue gas

Calculated data: Tnet = Net Temperature
 % CO₂ content in flue gas
 % Dry Flue Gas losses
 % Wet losses
 % Unburned carbon loss
 % Efficiency

$$\%CO_2 = (20.9 - \%O_2m) \times K2 / 20.9$$

$$Tnet = \text{Flue Temperature} - \text{Inlet Temperature}$$

$$\text{Dry flue gas loss} = 20.9 \times K1n \times (Tnet) / K2 \times (20.9 - \%O_2m)$$

$$\begin{aligned} \text{Wet loss simplified} &= 9 \times \%H_2 + \%H_2O / Qgr \times [2488 + 2.1Tf - 4.2 Ti] \\ &= [(9 \times \%H_2 + \%H_2O) / Qgr] \times 2425 \times [1 + 0.001 Tnet] \end{aligned}$$

$$\text{Wet loss} = K3(1+0.001xTnet)$$

$$\text{Where } K3 = [(9 \times \%H_2 + \%H_2O) / Qgr] \times 2425$$

$$\begin{aligned} \text{Net Efficiency} &= 100\% - \text{dry flue gas losses} \\ &= 100\% - 20.9 \times K1n \times (Tnet) / K2 \times (20.9 - \% O_2m) \end{aligned}$$

$$\begin{aligned} \text{Gross Efficiency} &= 100\% - \{\text{dry flue gas losses} + \text{wet losses}\} \\ &= 100\% - [20.9 \times K1g \times (Tnet) / K2 \times (20.9 - \%O_2m)] + \\ &\quad [K3 \times (1 + 0.001 \times Tnet)] \end{aligned}$$

$$\text{Excess Air} = [(20.9\% / (20.9\% - O_2m\%)) - 1] \times 100\%$$

$$CO_2\% = [(20.9\% - O_2m\%) \times K2\% / 20.9\%]$$

$$\text{Unburned fuel Loss} = K4 \times CO\% / (CO\% + CO_2\%)$$

Where K4 = 70 for coke
 = 65 for anthracite
 = 63 for Bituminous coal
 = 62 for coal tar fuel
 = 48 for liquid petroleum fuel
 = 32 for natural gas

The formula for K4 is based on the gross calorific value Qgr. To obtain the loss based on net calorific value multiply by Qgr/Qnet. Since this loss is usually small this conversion has been ignored.

$$\text{Oxygen Reference } CO(n) = CO \times \frac{(20.9 - O_2r)}{(20.9 - O_2m)}$$

D. CALCULATION OF FUEL DATA

For any fuel not specified by Kane International the net calorific value, gross calorific value and composition should be obtained from the fuel supplier.

The following fuel data has been calculated with reference to the efficiency calculation.

Example 1:

Chemical composition:	C	25%	
	H ₂	3%	
	H ₂ O	50%	
	Q _{net}	8.35 MJ/kg	
	Q _g	9.3 MJ/kg	*
	Max CO ₂	20.4%	

$$\begin{aligned} \mathbf{K1n} &= (255 \times \% \text{ carbon in fuel}) / Q_{\text{net}} \text{ (kJ/Kg)} \\ &= (255 \times 25) / 8350 = \mathbf{0.763} \end{aligned}$$

$$\begin{aligned} \mathbf{K1g} &= (255 \times \% \text{ carbon in fuel}) / Q_{\text{g}} \text{ (kJ/Kg)} \\ &= (255 \times 25) / 9300 = \mathbf{0.685} \end{aligned}$$

$$\mathbf{K2} = \text{Max \% CO}_2 = \mathbf{20.40}$$

$$\begin{aligned} \mathbf{K3} = \text{Wet Loss} &= [(9 \times \% \text{H}_2 + \% \text{H}_2\text{O}) / 9300] \times 2425 \\ &= [(9 \times 3 + 50) / 9300] \times 2425 \\ &= (77 / 9300) \times 2425 = \mathbf{20.08} \end{aligned}$$


$$\mathbf{K4} = \mathbf{65} \text{ (an approximation for wood) } *$$

The fuel values to program into the Analyser are as follows:

NATURAL GAS			
K1g	: 0.763	K1n	: 0.685
K_2	: 20.4	K_3	: 20.08
K_4	: 65	O2r	: 8.0

* Assumed values in the absence of supplied data. See previous appendix for other fuels.

E. ELECTROMAGNETIC COMPATABILITY (CE) STATEMENT

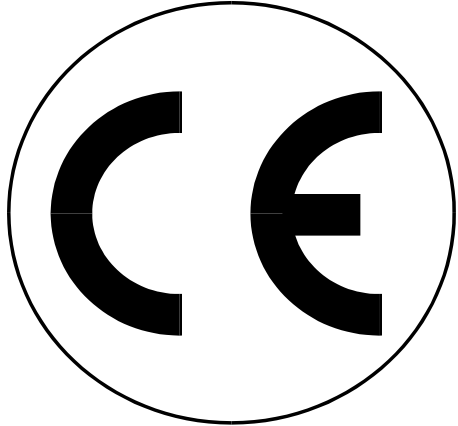

This product has been tested for compliance with the following generic standards:

EN 50081-1
EN 50082-1

and is certified to be compliant

Specification EC/EMC/KI/KM9106 details the specific test configuration, performance and conditions of use.



Thank you for reading this data sheet.

For pricing or for further information, please contact us at our UK Office, using the details below.



UK Office

Keison Products,

P.O. Box 2124, Chelmsford, Essex, CM1 3UP, England.

Tel: +44 (0)1245 600560

Fax: +44 (0)1245 600030

Email: sales@keison.co.uk

Please note - Product designs and specifications are subject to change without notice. The user is responsible for determining the suitability of this product.