


CERTIFIER[®] FA VENTILATOR TEST SYSTEMS

FOR GAS FLOW ANALYSIS

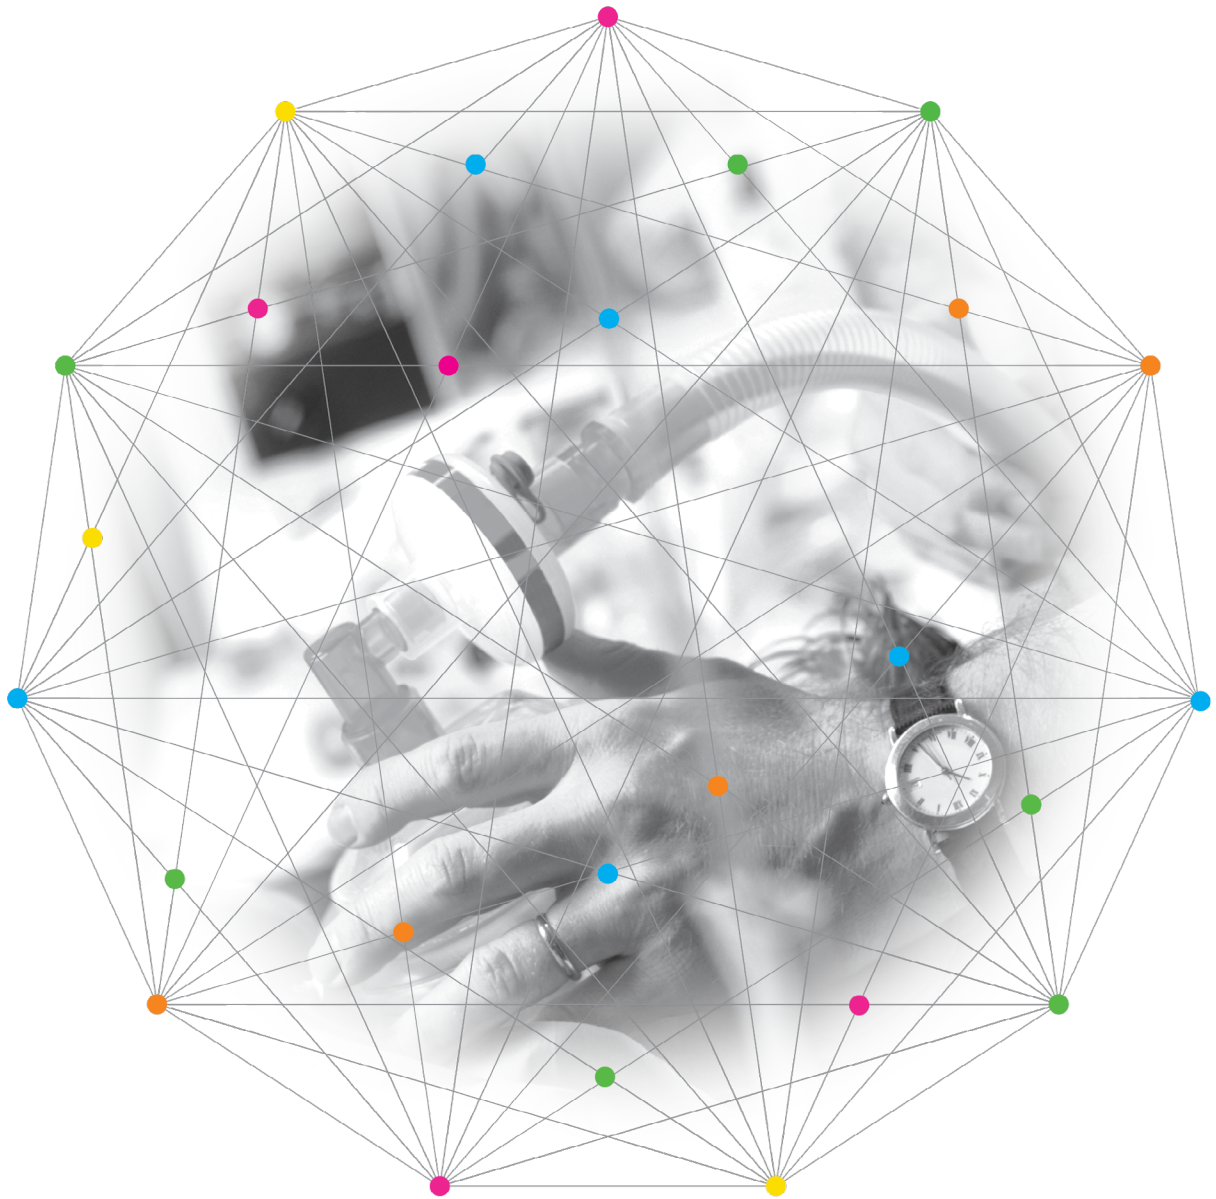

UNDERSTANDING, ACCELERATED

IDEAL FOR HOSPITAL, HOME-CARE, FIELD SERVICE, LABORATORY AND MANUFACTURING

CERTIFIER® FA PLUS VENTILATOR TEST SYSTEM


Certifier® FA Plus is the full-feature system capable of testing virtually all models of ventilators: adult, pediatric, anesthesia, neonatal and high-frequency.

Highlights


- + Color touch screen graphical user interface
- + Real-time graphing mode
- + Bi-directional flow measurement
- + Data storage using SD Flash card and internal memory
- + Stored data accessible through USB interface
- + Report printing capability
- + Rechargeable battery plus AC operation

Test Parameters


- + Flow
- + Peak & Minimum Flow
- + Volume (Inhaled and Exhaled)
- + Minute Volume
- + Low Pressure (Differential)
- + Peak & PEEP Pressure
- + Mean Airway Pressure
- + High Pressure
- + Barometric Pressure
- + Inspiratory Time
- + Expiratory Time
- + I:E Ratio
- + Respiratory Rate
- + Gas Temperature
- + Oxygen Concentration (with optional 4073 Kit)

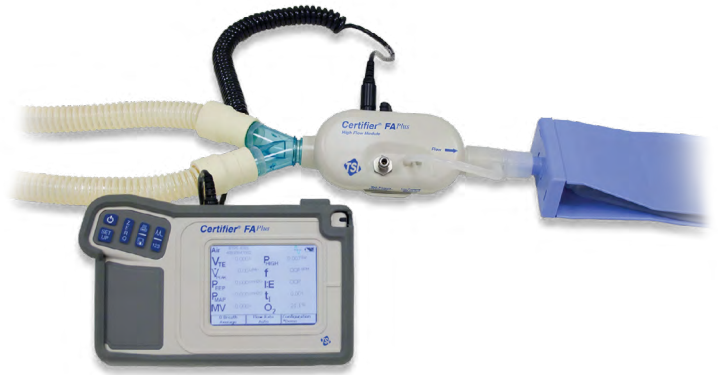

Features	Certifier FA Plus
Gas Calibrations	Air, O ₂ , Air/O ₂ mixtures, N ₂ , CO ₂ , N ₂ O
Flow Direction	Bi-Directional
Flow & Volume Modes	STP, ATP, BTPS, BTPD, plus user-defined
Temperature & Pressure Compensated	Yes
Max Breath Rate	1500 BPM
High Frequency Ventilators	Yes
High Pressure	-10 to 150 PSI (-.7 to 10 bar) Gauge
Low Pressure	-25 to 150 cm H ₂ O Differential
Barometric Pressure	7 to 25 PSIA (500 to 1700 mbar)
Display	Color-Graphic Touch Screen
Batteries	Li-Ion Rechargeable Battery Pack
AC Adapter	Yes
Internal Memory	1 MB
SD Flash Card	Included
Computer Interface	USB
Printing	USB

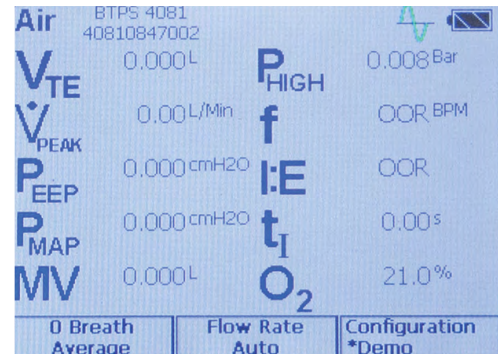

Displays up to 18 test parameters

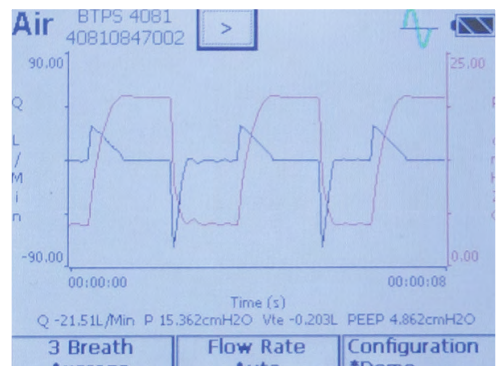

Graph up to 2 test parameters

CERTIFIER FA VENTILATOR TEST SYSTEM

Certifier FA is a low-cost test system capable of testing multiple parameters of ventilator performance.

Highlights

- + Simple, easy to read, user interface
- + Backlit LCD display
- + Entire kit weighs less than 3 lbs (1.4 Kg)
- + Volumes and flow in BTPS, ATP, or STP

Test Parameters

- + Flow
- + Peak Flow
- + Volume
- + Stacked Volume
- + Minute Volume
- + Low Pressure
- + Peak & PEEP Pressure
- + Barometric Pressure
- + Inspiratory Time
- + I:E Ratio
- + Respiratory Rate
- + Oxygen Concentration (with optional 4073 Kit)



Features	Certifier FA
Gas Calibrations	Air, O ₂ , Air/O ₂ mixtures, N ₂ O
Flow Direction	Uni-Directional
Flow & Volume Modes	STP, ATP, BTPS
Temperature & Pressure Compensated	Yes
Max Breath Rate	120 BPM
High Frequency Ventilators	-
High Pressure	-
Low Pressure	-25 to 150 cm H ₂ O Gauge
Barometric Pressure	7 to 30 PSIA (500 to 2000 mbar)
Display	Fixed Segment LCD
Batteries	4-AA Alkaline Batteries
AC Adapter	-
Internal Memory	-
SD Flash Card	-
Computer Interface	-
Printing	-



Displays 2 test parameters



4080 High-flow test system with
4082 Low-flow kit (sold separately)

Certifier FA Plus

	Gas/Mode	Range	Accuracy**
Flow-High Flow	Air, O ₂	-200 to +300 slpm*	±2% or ±0.075 slpm
	Air/O ₂ Mixtures	0 to 300 slpm	±4% or ±0.1 slpm
	N ₂	-200 to +300 slpm	±3% or ±0.1 slpm
	CO ₂	-40 to +40 slpm	±3% or ±0.1 slpm
Flow-Low Flow	Air, O ₂	0.01 to 20 slpm	±2% or ±0.01 slpm
	N ₂ , CO ₂	0.01 to 20 slpm	±3% or ±0.01 slpm
	N ₂ O	0.01 to 20 slpm	±4% or ±0.025 slpm
Volume-High Flow-Inhaled	Air, O ₂	0.01 to 10 liters STP	±2% Plus 0.02 liters
	Air/O ₂ Mixtures	0.01 to 10 liters STP	±4% Plus 0.02 liters
Volume-High Flow-Exhaled	Air, O ₂	0.01 to 10 liters STP	±3% Plus 0.03 liters
	Air/O ₂ Mixtures	0.01 to 10 liters STP	±4% Plus 0.04 liters
Volume-Low Flow-Inhaled	Air, O ₂	0.01 to 10 liters STP	±2% or ±0.01 liters
	N ₂ O	0.01 to 10 liters STP	±4% or ±0.01 liters
Minute Volume-High Flow	-	0.01 to 100 liters STP	±3%
Minute Volume-Low Flow	-	0 to 10 liters STP	±3%
Respiratory Times	Ti, Tip, Te	0.04 to 30 seconds	±2% or ±0.01 seconds
I:E Ratios	I:E, I:Eip	1:100 to 100:1	±4%
Respiratory Rate	f	1 to 1500 breaths per minute	±2% or 0.1 bpm
Low Pressure	All	-25 to +150 cm H ₂ O	±0.5% or ±0.15 cm H ₂ O
High Pressure	-	-10 to +150 PSI (-0.7 to 10 bar)	±1% or 0.1 PSI (7 mbar)
Barometric Pressure	-	7 to 23 PSI (500 to 1600 mbar)	±0.16 PSI (11 mbar)
Oxygen Concentration	-	21% to 100%	2% of concentration

* slpm = Standard Liters per Minute

** Accuracy stated as a percent of reading at TSI standard gas conditions.
See operators manual for more complete specifications

TSI and the TSI Logo are registered trademarks of TSI Incorporated.



4070 High-flow test system with
4073 Oxygen sensor kit (sold separately)

Certifier FA

	Gas	Range	Accuracy**
Flow-High Flow Module	Air, O ₂	0 to 300 slpm*	±2% or ±0.075 slpm
	Air/O ₂ Mixtures	0 to 300 slpm	±4% or ±0.1 slpm
Flow-Low Flow Module	Air, O ₂	0.01 to 15 slpm	±2% or ±0.01 slpm
	N ₂ O	0.01 to 15 slpm	±4% or ±0.025 slpm
Volume-High Flow-Inhaled	Air, O ₂	0.01 to 10 liters STP	±2% Plus 0.02 liters
	Air/O ₂ Mixtures	0.01 to 10 liters STP	±4% Plus 0.02 liters
Volume-Low Flow-Inhaled	Air, O ₂	0.01 to 9.999 liters STP	±2% or ±0.01 liters
	N ₂ O	0.01 to 10 liters STP	±4% or ±0.01 liters
Minute Volume-High Flow	-	0.01 to 99 liters STP	±7%
Minute Volume-Low Flow	-	0 to 9.999 liters STP	±7%
Inspiratory Time	-	0.25 to 60 seconds	±0.01 seconds
I:E Ratio-High Flow	-	1:100 to 100:1	±5%
I:E Ratio-Low Flow	-	1:15 to 15:1	±5%
Respiratory Rate	-	0.5 to 120 breaths per minute	±5%
Low Pressure	-	-25 to +150 cm H ₂ O	±0.75% or ±0.2 cm H ₂ O
Barometric Pressure	-	7 to 29 PSI (500 to 2000 mbar)	±0.16 PSI (11 mbar)
Oxygen Concentration	-	21% to 100%	2% of concentration

TO ORDER – CERTIFIER FA PLUS

Model Description
4080 High-Flow Standard Kit

Optional Modules and Accessories

Model Description
4073 Oxygen Sensor Kit
4082 Low-Flow Module

Part # Description
1208061 Extra battery pack and charger kit
1303860 Printer cable

TO ORDER – CERTIFIER FA

Model Description
4070 High-Flow Standard Kit

Optional Modules and Accessories

Model Description
4073 Oxygen Sensor Kit
4072 Low-Flow Module

Part # Description
1319288 Hard shell carrying case





Thank you for reading this data sheet.

For pricing or for further information, please contact us at our UK Office, using the details below.



UK Office

Keison Products,

P.O. Box 2124, Chelmsford, Essex, CM1 3UP, England.

Tel: +44 (0)330 088 0560

Fax: +44 (0)1245 808399

Email: sales@keison.co.uk

Please note - Product designs and specifications are subject to change without notice. The user is responsible for determining the suitability of this product.